

MagicSox: An E-Textile IoT System to Quantify Gait Abnormalities[☆]

Mohammadreza Abtahi^{a,b}, Joshua V. Gyllinsky^{a,b}, Brandon Paesang^{a,b},
Scott Barlow^a, Matthew Constant^{a,b}, Nicholas Gomes^a, Oliver Tully^a,
Susan D'Andrea^{a,c}, Kunal Mankodiya^{a,b,*}

^a*Department of Electrical, Computer and Biomedical Engineering,
University of Rhode Island, RI, USA, 02881.*

^b*Wearable Biosensing Lab, University of Rhode Island, RI, USA, 02881.*

^c*Providence VA Medical Center, Providence, RI, USA, 02908.*

Abstract

The global society is increasingly facing the challenges that reduce mobility, quality of life, and independence. Gait disorders are often both a result of, and predictor of further issues, tied to the 15 million stroke patients annually worldwide. These individuals face a number of gait abnormalities including drop foot that is a pathological condition, limiting patients' ability to lift the foot from the ground during the swing phase of walking. In this research work, we introduce a novel smart textile system, MagicSox that is woven with multiple sensors distributed over the surface of the foot. The overarching goal of MagicSox is to quantify the gait abnormalities in remote settings such as patients' homes so that clinicians and physical therapists can assess their patients on daily basis. The paper provides a detailed architecture of MagicSox that leverages the computing and communication capabilities of a modern Internet of Things (IoT) processor, the Intel Curie. We have developed an Android smart phone app that uses Bluetooth low energy (BLE) and automates the multi-sensor data collection from MagicSox. In terms of signal processing of wearable sensor data, we adopted multiplication of backward differences (MOBD) to analyze the multi-modal time series data to distinguish drop foot events from normal walking

[☆]This research is supported by the NSF Grants No. 1565962 and 1652538.

*Corresponding author

Email address: kunalm@uri.edu (Kunal Mankodiya)

cycles. We pursued a usability study on 12 healthy participants who were asked to walk normally and also to simulate drop foot cycles. We developed support vector machine (SVM) classifiers to analyze the data. The classification resulted in the accuracy of drop foot detection varying from 73.38% – 99.02%. The promising results now encourage us to evaluate MagicSox on stroke patients in future studies.

Keywords: Gait Abnormality, Wearable Sensors, IoT, E-Textile, SVM

1. Introduction

The global medical community is now attentive of Gait since the society witnesses the increasing population with decreased mobility due to medical conditions such as stroke, Parkinson’s, arthritis, and other age-related conditions [1, 2, 3]. The cyclic motion of gait biomechanics involves the entire body, providing an insight into a patient’s functional capabilities. A corpus of studies provide evidence that fluctuations in gait from one step to the other could reflect disruptions in intrinsic motor or postural control from age- or disease-related decline in the central and peripheral nervous systems [4, 5]. For example, the gait abnormality known as drop foot is described as an inability to lift the foot from the ground during the swing phase of the walking [6]. Drop foot could be a symptom of underlying disease or an effect of neurological conditions. With strokes affecting 15 million people globally each year and drop foot being a potential side-effect, it is a rising concern[7].

In this paper, we examine the use of smart textiles to measure the gait movements and differentiate between a healthy movement and a drop foot movement. People who have suffered from stroke pose as a great target group because of the sheer amount in society and their need for a cheaper and more efficient method of getting back on their feet. We have developed a smart textile called “MagicSox” to collect data on various attributes of motion on an individual’s lower extremities, designed to monitor patients with neurological diseases during their time of rehabilitation. MagicSox is embedded with a number of sensors

in various key locomotive points on the foot and ankle, strategically placed to measure movement, angle change, and forces exerted upon each step.

25 This research article provides an overall architecture of MagicSox (see Figure 1). The overarching goal of MagicSox is to automate the remote assessment of stroke patients, especially for gait rehabilitation. In addition to the on-board module consisting of multiple sensors and an Intel Curie microcontroller (with Bluetooth Low Energy(BLE)), MagicSox is embedded with algorithms such as
30 multiplication of backward differences (MOBD) to accurately differentiate between a standard walking step and a drop-foot step. We have pursued a usability study on 12 healthy participants who simulate drop foot gait during the data collection trial. The contribution of the paper is as following:

- Design and development of a smart textile system for remote drop foot
35 monitoring
- Selection and location of multiple motion sensors including flex sensor, pressure sensor, accelerometer and gyroscope
- Integration of the multiple sensors onto a textile material for quantifying foot locomotion
- 40 • Establishment of a signal processing algorithm (MOBD) to detect drop foot event
- Design of an Android app for patient-friendly data collection in remote settings
- Machine learning experimental analysis to measure the performance and
45 usability of MagicSox

The rest of the paper is organized as follows. In Section II, background and related works in gait abnormalities, drop foot and rehabilitation, and wearable biosensors for rehabilitation is discussed. In Section III, the design of MagicSox and the experiment setup are explained. In Section IV, we explain the methods

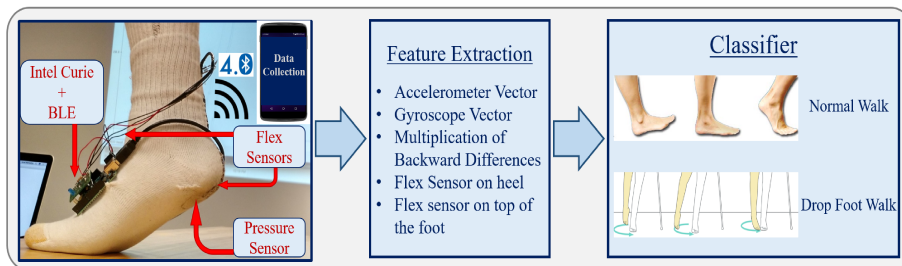


Figure 1: An overall system architecture of MagicSox.

50 we have used, in Section V we review and discuss our results, and in Section VI
 we conclude the paper.

2. Background and Related Works

2.1. Gait Abnormalities

Walking abnormalities, also referred to as gait abnormalities, are any abnormal
 55 or uncontrollable walking pattern. Factors causing gait abnormalities may
 include genetics, injuries or diseases afflicting the leg nerves, muscles or bones.
 The most common reasons that will lead to a gait abnormality include arthri-
 tis leg injuries, bone fractures, infections that damage tissues in the legs, shin
 splints (an injury common to athletes that causes pain in the shins), nervous
 60 system disorders such as cerebral palsy or stroke [8]. Therefore diagnosis of gait
 abnormality from observation can provide useful information regarding different
 neurological or musculoskeletal conditions.

In our research work, we focus on “drop foot” (also known as foot drop) that
 is not a disease but a type of gait abnormality that indicates someone’s inability
 65 to lift the front part of the foot [9]. This happens due to the weakness in the
 related muscles of lower limb. Drop foot is characterized by steppage gait [10].
 In this phase, the foot hangs down with the toes touching the ground. This
 causes the toes to scrape the ground while walking. Therefore, patients with
 drop foot usually lift their knees higher than usual or swing their leg in order
 70 to avoid dragging the toes on the ground.

Recently novel tools and technologies have been developed to improve the rehabilitation of patients with stroke [11], but they have not significantly impacted clinical practice. For this reason, some have suggested that home-based programs may be the answer [12].

75 Using wearable sensors and obtaining objective measures of gait and balance, will provide unique information of how and why the functional performance of gait and balance are impaired. Therefore, therapists can focus on the specific physiological reasons for difficulty in walking or balancing during specific tasks [13].

80 2.2. Wearable Technologies in Gait Rehabilitation

Smart wearable systems have great potential to be the future of healthcare tracking and can be used in a home based program. For example, Wang et al. [14] proposes a smart garment designed to monitor posture to support prevention and treatment of spinal pain during the neurological rehabilitation
85 of upper extremities. The garment combines various inertial measurement units that is controlled by an Arduino processor. The user will be notified that their posture is inadequate via internal vibration units along with alarms and visual instruction that is transmitted though Bluetooth to a smart phone.

S. Ryan Edgar et al. [15] and his research team developed a wearable shoe-
90 based rehabilitation monitoring device, designed specifically for stroke patients. The shoe is designed with an insole that has five pressure sensors integrated, in the heal part lies an insole connector that allows the microcontroller to read the shoes data. The actual shoe board is vertically placed along the backing of their shoe. The information is relayed to a phone from a Bluetooth mod-
95 ule. As well, the microcontroller contains a 3 – *axis* accelerometer to monitor directional motion. The smart phone application depicts the pressure exerted in each location on the soul of the foot as well as each axis reading from the accelerometer.

In another report by Mazzoldi et al. [16] wearable devices which are able
100 to read and record the posture and movements of a subject wearing the system

is discussed. The sensory function of the garments is achieved by fabric strain sensors, based on threads coated with polypyrrole or carbonloaded rubbers. The presence of conductive elements gives these materials piezoresistive properties, enabling the detection of local strain on the fabric.

105 In this research, we introduce MagicSox, a smart textile wearable device which can be used to quantify different aspects of gait abnormalities. Utilizing different types of sensors, will provide unique information regarding the orientation and angular velocity to understand the swing of the foot, pressure on the heel to better understand the heel strike and the angular displacement for
110 movement of the ankle for dorsiflexion. In addition to aiding the stroke rehabilitation process, MagicSox is also a healthcare tool for everyday life. It can be used to provide insights for athletes or to aid in posture.

3. Design

3.1. *MagicSox*

115 MagicSox is a smart textile system with Internet-of-Things (IoT) functionalities to sense, compute and communicate the gait abnormalities such as drop foot. Our design utilizes four different types of sensors, measuring force, resistance, orientation, and angular velocity. With a total of five sensors, two of which built in to our microcontroller, they provide the data that allow us to
120 differentiate normal walking from gait abnormalities.

- Arduino 101 board with the Intel Curie processor module
- Gyroscope and Accelerometer integrated in the Intel Curie
- Pressure Sensor on the heel
- 2 Flex Sensors, one along the heel and the other one on the anterior side
125 of the ankle
- Smart Phone to collect the data via Bluetooth in the application

3.1.1. Inertia Measurement Units

The Arduino 101 has an on-board 6-axis accelerometer/gyroscope. The microcontroller measures orientation with its accelerometer and angular velocity with its gyroscope. In unison, they form an inertial monitoring unit (IMU) that allow us to read the kinematics behind the foot. Once data collection begins on the Arduino, the gyroscope raw values are converted into an angular velocity for each of the three axes (g_x, g_y, g_z). Similarly, the accelerometer measures the acceleration for each axis (a_x, a_y, a_z), returning a raw value in need of conversion. The gyroscope is useful because of its ability to measure rotational movement around the axes. The accelerometer does not have this function if the movement remains continuous. These sensors can show how much a person takes their foot up in order to complete the gait cycle. Also, they can show if the person swings their foot while walking which is a normal symptom in the drop foot phenomena. As an example, Figure 2 shows the data from the gyroscope, and the zoomed-in picture to observe the difference between normal walk and drop foot walk, respectively. As shown in Figure 2, accelerometer and gyroscope are located on top of the foot.

3.1.2. Pressure Sensor

The Arduino IMU reads kinematic data for our sock. Additionally we use a pressure sensor to detect when the individual wearing the sock has a definitive heel strike vs. a standard step. Heel striking is of critical concern to athletes and is well documented in athletic literature [17, 18, 19]. However, we hypothesize that heel striking could be an important feature to consider in drop foot analysis. We used the FlexiForce A201 [Tekscan, 9.7mm in diameter] that is a piezoresistive sensor, made of a semiconductor material. The pressure sensor acts as a pressure sensing resistor in an electrical circuit. Beneath the sensors film and adhesives lies a silver strip and pressure sensitive ink. The active sensing area is only where the silver is in contact with the ink. When force is applied to the sensor, the resistance decreases. When the force is removed, the resistance is very high. The FlexiForce sensor is thin enough to allow non-intrusive

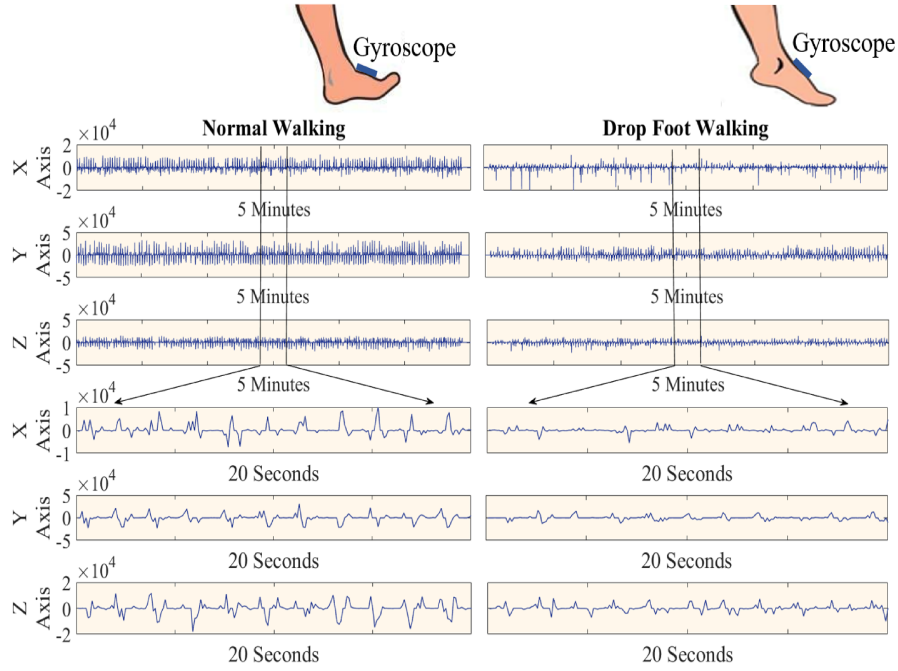


Figure 2: Gyroscope data for Normal and Drop Foot walking. 5 minutes data in top 3 panels and 20 seconds zoomed in data in bottom 3 panels.

measurement, fitting for our smart textile design. In our experiment, the sensor is located on the heel portion of the sock as shown in Figure 1.

160

3.1.3. Flex Sensor

The flex sensor is aimed at measuring angular displacement at the ankle joint. Flex sensors are analog resistors that act as variable analog voltage dividers. Under the flexible substrate of the sensor lies carbon resistive elements. As the substrate is bent, the sensor creates resistance output that is similar to the radius of the bend. In our design, we use the Spectra Symbol flex sensor that has a thickness of $6.35mm$, with 84.86% of the part length designated as active length. While lying flat, it has a resistance of $7K$ to $13K$ ohms. Its bent resistance is minimally two times greater than the flat resistance at a 180

165

170 degrees pitch bend. The sensor takes use of an impedance buffer and voltage divider, contributing to a reduced error.

We have used two flex sensors, one located on the heel along with the pressure sensor, and the other one is located in the anterior side of the foot on the ankle. These locations have been chosen in order to estimate that how normally the
175 person can complete a gait cycle. In the area of stroke rehabilitation, these sensors will provide information regarding the ankle dorsiflexion. Since one of the exercises in the stroke rehabilitation is ankle dorsiflexion, these sensors can show the strength and duration of this exercise. They also can provide the difference between the normal gait and the drop foot gait, because the ankle
180 flexion is reduced in the drop foot gait compared to the normal gait. Figure 3 shows the data from flex sensor located on the heel and the zoomed in picture of it. Each of the peaks is a step and the difference between normal and drop foot walk is clearly visible in both amplitude and duration. The location of the flex sensor in determined on the foot on top of the figure.

185

3.1.4. Intel Curie Microcontroller with BLE

All the sensors are connected to the microprocessor board Arduino 101, which collects the data from the pressure and flex sensors, utilizing its built-in accelerometer and gyroscope as well. All the data from the Arduino board is
190 sent to MagicSox application on the smart phone. MagicSox application was designed to run on any Bluetooth Smart or Bluetooth Smart Ready enabled device running Android 4.4 or higher. This Android device utilizes the BLE technology available on both the Arduino 101 and the device itself to receive updates every 100 milliseconds from MagicSox. This update comes in the form
195 of a byte array which contains all the essential information from MagicSox, including raw sensor data from the two Flex Sensors, the Pressure Sensor, the Accelerometer and the Gyroscope. The Android device then parses this data and saves all of it into a Comma Separated Values (CSV) file which can be used for further processing later. Figure 4 shows how MagicSox application works on

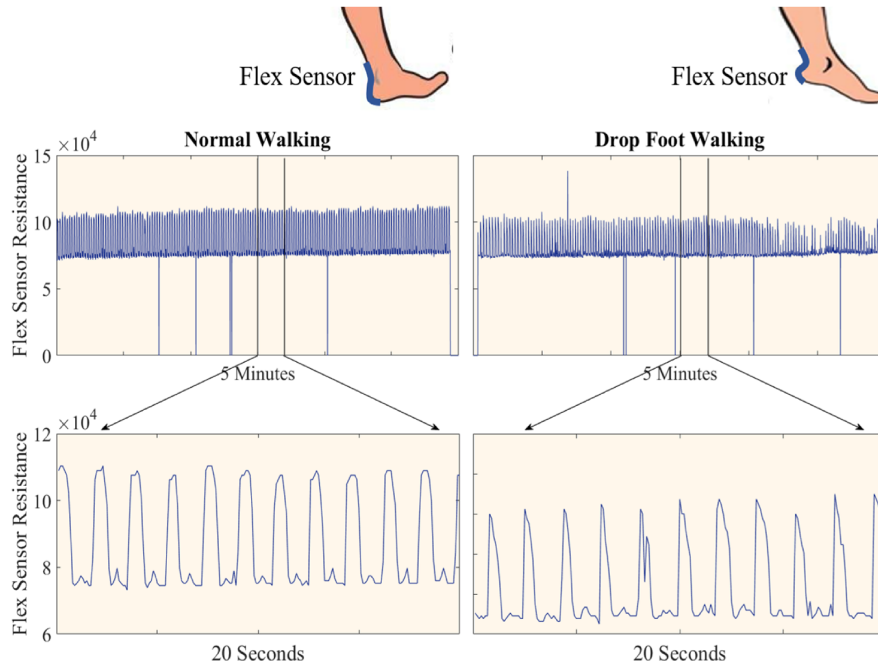


Figure 3: The data from the flex sensor located on the heel. 5 minutes data in top panels and zoomed in 20 seconds data in bottom panels. The visual observation of the flex sensor data provides an understanding of how drop foot differs from normal walking. In each walking cycle, the ankle dorsiflexion in drop foot is weak.

200 the smart phone.

3.1.5. E-Textile Design Configurations

The first batch of socks attached the microcontroller directly to the sock, stitching at the grounding screw-holes. Due to the Printed Circuit Board (PCB) layout of the Arduino 101, the attachments were not equidistant and there was a slight overhang of the board from the attachment locations which was
 205 inconsistent across among the four points. This lopsided method was sufficient for early experimentation, but did not provide an ideal long-term solution.

The second batch of socks produced for the experiment were modified slightly to take advantage of insight gained in the initial round. None of the electronic or
 210 sensor layout was changed among the versions, merely the attachment methods.

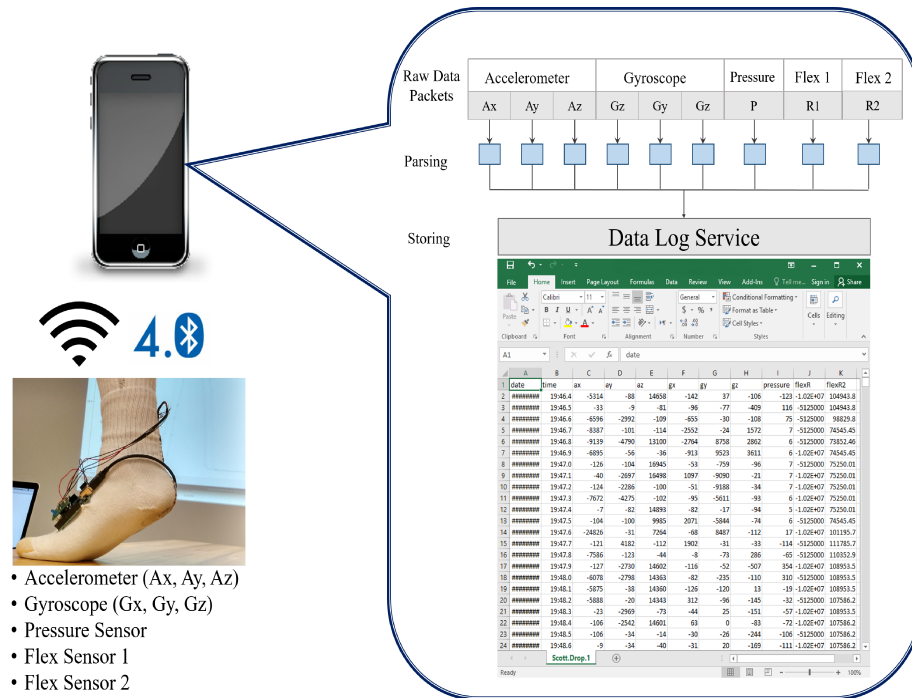


Figure 4: An operational flow chart of the Android smart phone app.

These improvements enabled more stable experiments with rough users. Instead of directly attaching the microcontroller’s PCB onto the socks at the point of attachment being the ground in screws, a 3D printed base was developed to act as an interface between the microcontroller and the fabric. The plastic acted as a minimalistic anti-static shield. The 3D printed Bates with stitched onto a Velcro attachment which allowed the joining of the curved and flat surface more easily.

Sensor sleeves were constructed using a stretchy mesh netting material. The textile pattern was tailored to the various sensors dimensions, using a 0.25 of an inch seam allowance. The pattern was based on a modified standard large men’s sock. Due to the difficulty in sewing such pliable fabric, we pinned the cut mesh sleeve onto tear away paper in order to prevent gathering or from moving

around as it was sewed onto the sleeve. Each sensor was placed into the sleeve and hand stitched on top to enclose and lock the sensor into the sleeve. During attachment to the sock, the side seam was reopened to enable flat sewing, with chock contours guides determined first on a model. Slits were cut in the material and the sensors were channeled through them at each location, including the dorsum of the foot, heel and ankle. Pressure and flex sensors were attached using a $2mm$ stitch length. The pressure sensor was placed on the heel. Flex sensors were placed on top of the foot at the arch. We then hand stitched Velcro to a 3D printed PCB mount using Velcro and stitched a Velcro strap to the sock in order to attach the PCB to the sock itself. After sewing all the sensors and Velcro to the sock, the raw cut edges of the sock were reattached with a double stitch using the least amount of seam allowance possible with the fabric inside out. Figure 5 shows the design iterations and improvements of the MagicSox.

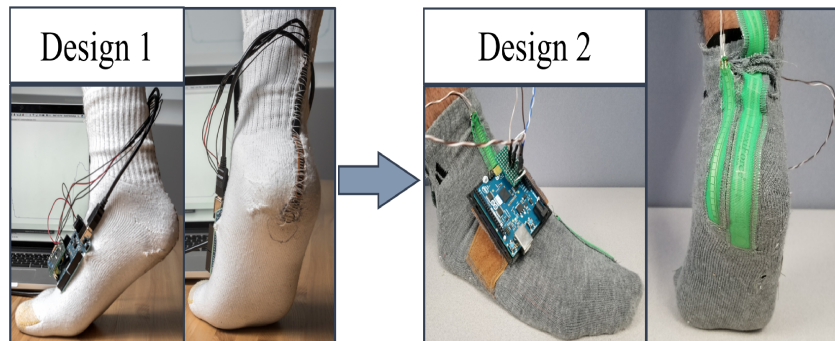


Figure 5: Design iterations of the MagicSox. The sensors and the microcontroller were stitched directly to the sock in the Design 1, but sensor sleeves were used in the Design 2. Also, the microcontroller is attached to the socks via velcro and a 3D printed shield.

3.2. Experimental Setup

The main goal of this paper is to distinguish between the normal gait and the drop foot which, as mentioned earlier, is a gait abnormality caused by stroke that happens because of the damage to the fibular nerve, sciatic nerve and muscles in the anterior side of the lower leg.

In order to collect the data, we recruited 12 healthy subjects to walk in two different situations, one is the normal gait and the other one is to simulate the drop foot walking. The first 4 participants were asked to do the experiment with the first batch of socks and the remaining 8 participants performed the
245 experiment with the newer version of the socks in order to compare the different versions of the sock and observe how design developments can change the results. Both groups performed the same two walking tests. Each participant was asked to walk for 5 minutes in their normal gait and afterwards, they were asked to simulate the drop foot walking for 5 minutes. Therefore, we have an overall of
250 10 minutes of data from each participant which is separated equally into normal gait and drop foot walking.

The data has been recorded from the accelerometer, gyroscope, pressure sensor and two flex sensors. As mentioned previously, the flex sensors and the pressure sensors are variable resistances. Static state for relativity is required
255 to measure this physical state. We accomplish this static state by introducing a standard resistor. To measure the relative change in state between the standard resistor and flex or pressure sensors, we designed a voltage divider that allows us to extrapolate the desired information using Ohm's Law. One last challenge on this setup is maximizing the voltage range to increase the signal to noise
260 ratio. We chose to use a standard $10k\Omega$ resistor, which provides a potential voltage swing of approximately $1v$. Therefore, the data that is recorded from the pressure sensor and two flex sensors are the voltage across these sensors. Since the accelerometer and gyroscope each have 3 different dimensions, we have an overall of 9 attributes in the data. The data is recorded continuously
265 via Bluetooth to a smart phone by the sampling frequency of $10Hz$ for each data channel.

4. Methods

4.1. Support Vector Machine (SVM)

After collecting the data, in order to distinguish between the normal gait
270 and drop foot walking, we used a Support Vector Machine (SVM). The SVM
uses a nonlinear mapping to transform the original training data into a higher
dimension. It searches for the linear optimal separating hyperplane in this new
dimension (that is, a “decision boundary” separating the tuples of one class
from another). With an appropriate nonlinear mapping to a sufficiently high
275 dimension, data from two classes can always be separated by a hyperplane [20].
SVMs are supervised learning models.

The general concept of the SVM is that the system trains itself based on a
training dataset which can be a part of the original dataset that is labeled into
two different categories. Then, after the system is trained, it will be tested on
280 the other part of the original dataset to predict the labels of the data, and by
comparing the predicted labels and the original labels, we can find the accu-
racy of the system. In this study, we used several learning algorithms to be
implemented in the SVMs. It is possible to classify the datasets which are not
linearly separable by applying the Lagrangian optimization theory to a linear
support using the Kernel. While the nonlinear support vector machines retain
285 the efficiency of finding linear decision surfaces, they allow us to apply them to
not linearly separable datasets. It is also possible to change the margins of the
classifiers and change the complexity and accuracy of the systems. In general,
large margins make the system less complex, but on the other hand, will let the
290 system generate more errors, resulting to lower accuracy. This can be achieved
by changing a variable called Cost constant in the classifier models.

Figure 6 shows a concept of the SVM and its supporting hyperplanes that di-
vide two different classes and introduces the margin. When we make the margin
large, we allow some data points between the decision surface and the support-
295 ing hyperplanes, which at the end will result in false classification and reduce
the accuracy.

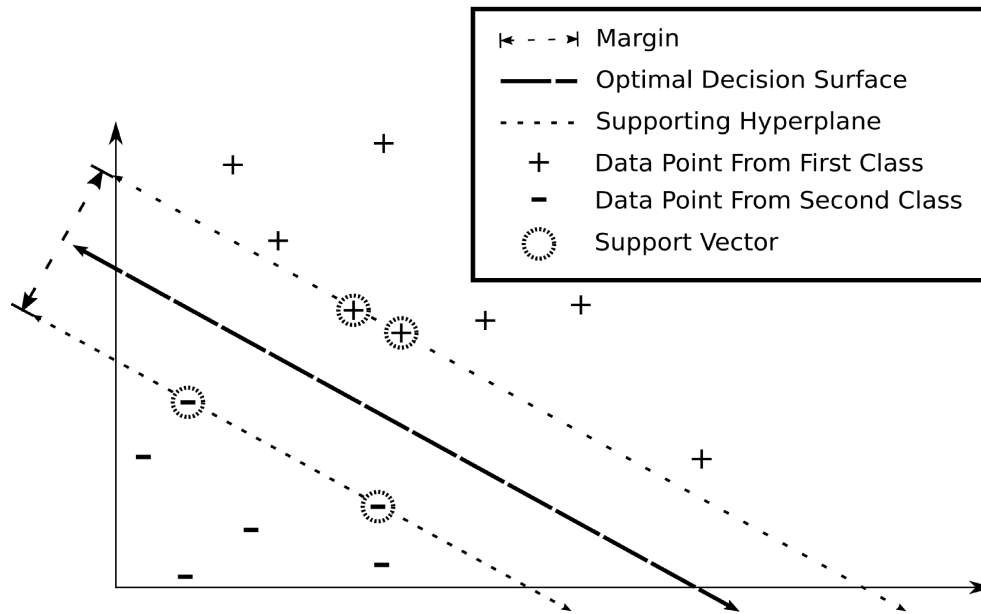


Figure 6: A concept of SVM and the terms of decision surface, supporting hyperplane and margins.

Different types of SVM classifiers are applied on the data in order to compare their performance. We have used 4 different types of Kernel functions all of them with 3 different Cost constants of 1, 10 and 100. Table 1 shows different learning algorithms that have been used in this study with their complexity index which we will refer to them later in the results section.

Table 1: Different methods of classification used in this study.

Index	Kernel Name	Kernel Function	Degree	Cost Constant
1	Linear Kernel	$k(\vec{x}, \vec{y}) = \vec{x} \cdot \vec{y}$	-	1
2	Linear Kernel	$k(\vec{x}, \vec{y}) = \vec{x} \cdot \vec{y}$	-	10
3	Linear Kernel	$k(\vec{x}, \vec{y}) = \vec{x} \cdot \vec{y}$	-	100
4	Polynomial Kernel	$k(\vec{x}, \vec{y}) = (\vec{x} \cdot \vec{y} + c)^d$	d=2	1
5	Polynomial Kernel	$k(\vec{x}, \vec{y}) = (\vec{x} \cdot \vec{y} + c)^d$	d=2	10
6	Polynomial Kernel	$k(\vec{x}, \vec{y}) = (\vec{x} \cdot \vec{y} + c)^d$	d=2	100
7	Polynomial kernel	$k(\vec{x}, \vec{y}) = (\vec{x} \cdot \vec{y} + c)^d$	d=3	1
8	Polynomial Kernel	$k(\vec{x}, \vec{y}) = (\vec{x} \cdot \vec{y} + c)^d$	d=3	10
9	Polynomial kernel	$k(\vec{x}, \vec{y}) = (\vec{x} \cdot \vec{y} + c)^d$	d=3	100
10	Radial kernel	$k(\vec{x}, \vec{y}) = e^{-(\vec{x} - \vec{y} ^2 / 2\sigma^2)}$	-	1
11	Radial kernel	$k(\vec{x}, \vec{y}) = e^{-(\vec{x} - \vec{y} ^2 / 2\sigma^2)}$	-	10
12	Radial Kernel	$k(\vec{x}, \vec{y}) = e^{-(\vec{x} - \vec{y} ^2 / 2\sigma^2)}$	-	100

Regarding the evaluation of the methods, we used 2 different evaluation methods of 10-Fold Cross-Validation and Hold-Out method with the portion of 2/3 and 1/3 for training and evaluating respectively.

305 In this paper, we provided the raw data recorded from all the sensors to the classifier and compared the performance with the case where we used the Multiplication of Backward Differences (MOBD) algorithm for the data recorded from the pressure sensor which is a useful tool to determine the heel strike. Determining the heel strike is useful here because in the drop foot walking, the
310 heel strike happens less or with a lower pressure compared to the normal gait.

4.2. Multiplication of Backward Differences (MOBD)

The MOBD algorithm was developed in the efforts to create a better method for detection of the large spikes in heart wave signal [21, 22]. Using the MOBD algorithm for heel strike detection seemed applicable due to the fact that the
315 spike in heart wave and the impact transient of heel strike share that similar sharp waveform.

The algorithm computes a backward derivative which in discrete time, a derivative is well approximated by a difference. Those differences are then multiplied together, which in turn provides a robust peak detector.

Assuming $p[n]$ be the pressure sensor data in time sample n , the first-order backward difference at time n , $x[n]$, is:

$$x[n] = p[n] - p[n - 1] \quad (1)$$

Therefore, the $N - th$ order MOBD nonlinear transform is as follow:

$$y[n] = \prod_{k=0}^{N-1} |x[n - k]| \quad (2)$$

Also, $y[n]$ is forced to be zero if the backward differences are not in agreement with respect to sign.

$$y[n] = 0, \text{ if } \text{sgn}(x[n - k]) \neq \text{sgn}(x[n - (k + 1)]) \text{ } k = 0, 1, \dots, N - 2$$

where the $\text{sgn}(x)$ is the signum function.

At a given time, a sample from the pressure sensor is stored in the micro-
320 controller. At the next sample time, another sample from the sensor is stored. Those two samples are then subtracted and stored in its own variable. This is then repeated two more times so that 3 differences have been collected. The algorithm then checks for 3 consecutive positive or negative differences. When climbing up a steep waveform, a peak, the algorithm will result in consecutive
325 differences in comparison to a waveform that has a more rounded shape to it. If 3 consecutive differences are found, they are multiplied together and that value is compared to a predefined threshold value. If the calculate value is greater than the threshold value, the algorithm recognizes the detection of a heel strike.

The impact values of a heel strike are much larger than that of a non-heel
330 strike impact due to the distributions of forces along the foot for each strike. A threshold value was determined that allowed for the heel strike impact transient to be detected while avoiding possible false peaks that could stem from various

types of noise. Figure 7 shows the data from the pressure sensor along with the MOBD results. The MOBD algorithm output would be 1 if it detects a heel strike and 0 if there is no heel strike. As it can be seen from Figure 7, we have
 335 heel strike for normal walking, but no heel strike for drop foot walking.

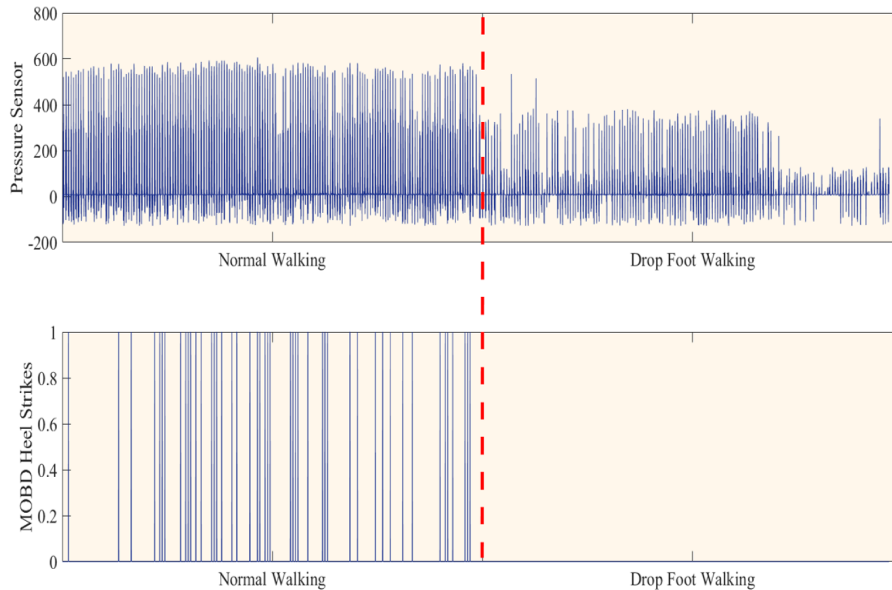


Figure 7: The raw data from the pressure sensor (top panel) and the MOBD algorithm results showing the heel strike (bottom panel).

4.3. Evaluation

Recalling from the explanation of the support vector machine, it needs to divide the original dataset into two parts; one for training itself and one for testing and providing the accuracy, which is called evaluation. On the evaluation
 340 aspect of the classification, we used two different methods of training and testing the system which are Hold-Out and k -Fold Cross-Validation. The Hold-Out method simply takes one portion of the dataset for the training and holds the other portion for testing the accuracy. The ratio of these portions can be defined
 345 by the user and we defined the portions to be $2/3$ and $1/3$ for training and testing, respectively. In k -Fold Cross-Validation, the system divides the dataset

into k different folds which the length of each fold is the same as the others and no folds have overlap with each other. The concept is that the system uses each of these folds for testing while getting trained from the other folds, and
350 at the end, provides the accuracy of the system which is the average of all the accuracies on different folds. In this paper we used the Hold-Out method with the portions to be $2/3$ and $1/3$, and k -Fold Cross-Validation with the number of folds k equal to 10.

5. Results and Discussion

355 In this section, we report the results of the classification of the normal walking and the drop foot walking and compare the performance of the classifier for the two cases mentioned earlier.

1. Classifying the raw dataset

In this case, we labeled the data to 0 and 1 for the normal and drop foot
360 walk respectively and without any processing, sent the raw data to the classifier. Table 2 shows the performance of different SVM and evaluation methods applied on the raw data.

2. Classifying the feature extracted dataset

In this case, we first applied the MOBD algorithm as explained in the
365 previous section in order to apply different types of SVM classifiers. The new dataset contains all the previous information, except the pressure sensor data which is replaced by the results of MOBD algorithm.

After applying the MOBD algorithm and labeling the data to 0 and 1 for the normal walking and drop foot walking respectively, we applied
370 the dataset to the classifier in order to observe the performance. Table 3 shows the accuracy of different SVM and evaluation methods applied on the feature extracted dataset.

As it can be seen from Tables 2 and 3, the performance of the system improves as we use more complex Kernel functions such as the Radial kernel or

Table 2: The performance of different methods on the raw data from each of the participants.

Index	Evaluation	MagicSox Design 1				MagicSox Design 2							
		P1	P2	P3	P4	P5	P6	P7	P8	P9	P10	P11	P12
1	Hold-Out	63.16%	94.02%	53.93%	56.29%	82.91%	72.31%	76.53%	68.74%	72.36%	78.14%	80.09%	59.47%
	10 Fold	63.46%	93.56%	51.39%	55.92%	82.49%	71.01%	76.17%	68.85%	72.41%	77.93%	80.03%	59.64%
2	Hold-Out	63.16%	95.03%	53.93%	56.29%	82.85%	72.36%	77.03%	69.92%	73.14%	79.26%	80.77%	59.47%
	10 Fold	63.47%	94.69%	51.41%	55.62%	82.28%	71.24%	76.90%	69.75%	73.10%	78.83%	80.26%	59.66%
3	Hold-Out	62.80%	94.93%	54.08%	56.29%	82.85%	72.31%	77.19%	70.28%	73.84%	79.93%	81.14%	60.03%
	10 Fold	56.00%	94.68%	50.83%	56.02%	82.33%	71.14%	77.09%	70.14%	73.56%	79.22%	80.94%	60.14%
4	Hold-Out	70.07%	87.58%	56.64%	57.19%	93.36%	84.16%	83.52%	79.24%	80.73%	88.47%	89.06%	73.13%
	10 Fold	68.96%	86.83%	57.01%	58.08%	93.10%	84.18%	83.57%	79.02%	80.12%	87.98%	88.53%	73.24%
5	Hold-Out	68.50%	87.78%	56.34%	57.75%	94.25%	85.58%	83.47%	79.58%	80.82%	88.33%	88.92%	74.05%
	10 Fold	68.93%	86.94%	57.59%	58.05%	94.91%	85.43%	83.52%	79.46%	80.34%	88.09%	88.51%	73.91%
6	Hold-Out	68.34%	87.88%	56.34%	57.70%	95.19%	86.83%	85.14%	81.39%	81.97%	89.46%	91.15%	76.32%
	10 Fold	68.78%	86.94%	57.46%	58.02%	95.48%	85.99%	85.73%	81.65%	82.19%	89.07%	90.74%	77.20%
7	Hold-Out	72.36%	88.19%	65.36%	60.01%	92.78%	87.09%	83.96%	81.06%	81.44%	88.47%	91.07%	78.51%
	10 Fold	72.52%	87.61%	64.73%	61.34%	96.75%	87.96%	84.01%	80.97%	81.73%	88.39%	90.83%	79.04%
8	Hold-Out	72.00%	92.60%	81.20%	61.62%	97.28%	90.22%	86.72%	83.71%	83.16%	90.07%	92.12%	80.02%
	10 Fold	73.03%	92.22%	69.04%	62.93%	97.78%	91.37%	86.54%	83.48%	82.97%	89.73%	91.89%	79.97%
9	Hold-Out	71.59%	94.17%	82.91%	61.42%	97.69%	93.67%	87.19%	84.42%	84.41%	91.23%	92.84%	80.84%
	10 Fold	73.22%	94.94%	73.26%	63.33%	98.24%	94.11%	87.33%	85.01%	84.29%	91.19%	92.47%	80.47%
10	Hold-Out	75.30%	95.79%	74.23%	65.69%	98.48%	93.68%	87.42%	85.72%	86.10%	91.96%	92.60%	79.19%
	10 Fold	76.30%	95.71%	76.95%	67.41%	98.65%	94.25%	87.47%	85.87%	85.97%	92.01%	91.94%	78.93%
11	Hold-Out	75.35%	98.63%	88.67%	71.43%	98.90%	95.35%	89.19%	86.43%	87.49%	92.65%	93.69%	80.92%
	10 Fold	76.38%	98.19%	89.42%	73.25%	98.86%	95.94%	88.97%	86.37%	87.21%	92.84%	92.19%	79.48%
12	Hold-Out	76.12%	98.68%	89.07%	73.44%	98.79%	96.34%	92.06%	89.74%	89.94%	94.15%	95.02%	82.06%
	10 Fold	76.45%	98.38%	89.69%	74.37%	98.98%	96.36%	91.88%	89.91%	89.87%	94.71%	94.55%	81.93%

375 Polynomial Kernel with degree 3, and results in the accuracy of almost more than 80% for all the participants with the Radial Kernel function and the Cost constant of 100. Figure 8 shows a comparison of the performance of the best model which is the SVM with Radial Kernel and Cost constant of 100 evaluated with the Hold-Out and 10-Fold Cross-Validation methods for all participants applied to both raw dataset and feature extracted dataset. It can be seen from the results that using the raw dataset and the feature extracted dataset will lead to almost same performance of the classifier. It was also noticed that the 2 different evaluation methods of Hold-Out and 10-Fold Cross-Validation have similar performance on the data, therefore, choosing either one will result in mostly the same result. It is apparent from the results that the design improvements for the socks will result in better performances. It can be seen that the results for participants 5 to 8 are more consistent and provide higher accuracies

380

385

Table 3: The performance of different methods on the features extracted data from each of the participants.

Index	Evaluation	MagicSox Design 1				MagicSox Design 2							
		P1	P2	P3	P4	P5	P6	P7	P8	P9	P10	P11	P12
1	Hold-Out	63.31%	93.30%	52.48%	54.32%	82.85%	72.04%	76.37%	68.59%	72.19%	77.95%	79.84%	60.14%
	10 Fold	63.46%	93.54%	51.93%	55.55%	82.33%	71.83%	76.04%	68.63%	72.28%	77.43%	79.80%	59.86%
2	Hold-Out	63.41%	94.77%	52.48%	54.38%	82.85%	72.05%	76.91%	68.59%	73.10%	79.10%	80.23%	60.14%
	10 Fold	63.41%	94.18%	51.48%	55.94%	82.37%	71.82%	76.83%	68.84%	73.19%	78.77%	80.09%	60.03%
3	Hold-Out	64.32%	94.72%	52.48%	54.38%	82.90%	71.99%	77.01%	70.12%	73.77%	79.84%	80.97%	60.74%
	10 Fold	65.90%	94.17%	51.86%	55.94%	82.31%	71.57%	76.902%	70.01%	73.43%	79.09%	80.71%	60.62%
4	Hold-Out	72.30%	86.36%	54.98%	54.17%	90.38%	81.03%	83.40%	79.32%	80.71%	88.31%	88.12%	72.85%
	10 Fold	72.82%	86.59%	53.31%	55.65%	92.05%	82.06%	83.52%	79.24%	80.01%	87.90%	87.74%	72.64%
5	Hold-Out	70.32%	86.06%	54.33%	55.13%	95.66%	86.52%	83.59%	79.63%	80.89%	88.30%	88.63%	73.84%
	10 Fold	71.34%	86.29%	53.90%	55.80%	95.71%	87.33%	83.61%	79.56%	80.33%	88.01%	88.19%	73.69%
6	Hold-Out	69.97%	85.90%	55.04%	55.53%	97.64%	91.58%	85.22%	81.33%	82.01%	89.29%	90.92%	75.15%
	10 Fold	70.88%	86.05%	54.28%	56.05%	96.86%	90.17%	85.91%	81.58%	81.94%	88.82%	89.48%	75.94%
7	Hold-Out	70.22%	87.38%	55.59%	59.15%	93.93%	85.47%	83.91%	81.12%	81.25%	88.71%	90.46%	77.14%
	10 Fold	71.20%	87.46%	58.63%	61.65%	96.46%	85.59%	83.97%	81.09%	81.70%	88.25%	89.73%	78.01%
8	Hold-Out	73.32%	91.48%	65.26%	60.96%	97.07%	92.42%	85.92%	83.46%	83.19%	89.93%	91.83%	79.27%
	10 Fold	73.86%	91.73%	68.51%	62.56%	97.12%	91.46%	86.47%	83.31%	83.02%	89.55%	91.71%	79.19%
9	Hold-Out	75.86%	91.58%	69.52%	62.37%	97.33%	93.67%	87.10%	84.20%	84.39%	91.15%	92.35%	80.20%
	10 Fold	76.09%	92.66%	71.47%	64.36%	97.63%	93.01%	87.24%	84.89%	84.21%	90.97%	91.99%	79.97%
10	Hold-Out	76.01%	91.94%	72.33%	63.53%	98.41%	95.14%	87.29%	85.69%	85.98%	91.59%	92.47%	80.05%
	10 Fold	76.42%	93.25%	75.48%	67.57%	98.57%	94.28%	87.33%	85.85%	85.91%	91.64%	92.04%	79.12%
11	Hold-Out	77.03%	94.78%	87.67%	73.04%	98.64%	96.55%	89.27%	86.41%	87.33%	92.49%	93.48%	80.74%
	10 Fold	76.06%	95.60%	88.98%	73.19%	99.02%	95.97%	89.05%	86.39%	87.15%	92.63%	92.23%	79.57%
12	Hold-Out	75.81%	95.64%	87.97%	73.39%	98.95%	96.76%	91.94%	89.88%	89.75%	94.06%	94.76%	81.97%
	10 Fold	76.88%	95.89%	88.65%	73.38%	98.90%	96.24%	91.90%	89.73%	89.81%	94.58%	94.51%	81.89%

compared to the first 4 participants. The first version of the socks provided the average accuracy of 83.98% among all four participants, compared to the newer
390 version of the socks with the average accuracy of 92.24% among the rest of the participants.

As an example of the performance of the classifier, we show the actual labels and predicted labels of the classifier applied to the whole length dataset of one of the participants in Table 4. The table shows that we have 838 False Positives
395 and 146 False Negatives. Figure 9 shows a visual representation of the table for the first 600 samples and the zoomed-in picture of 50 samples. The white color represent label 0 as normal walking, the blue color represents label 1 as drop foot walking and the red color shows the error of the system in prediction, which means that the actual labels are 0, but the classifier predicts them as 1

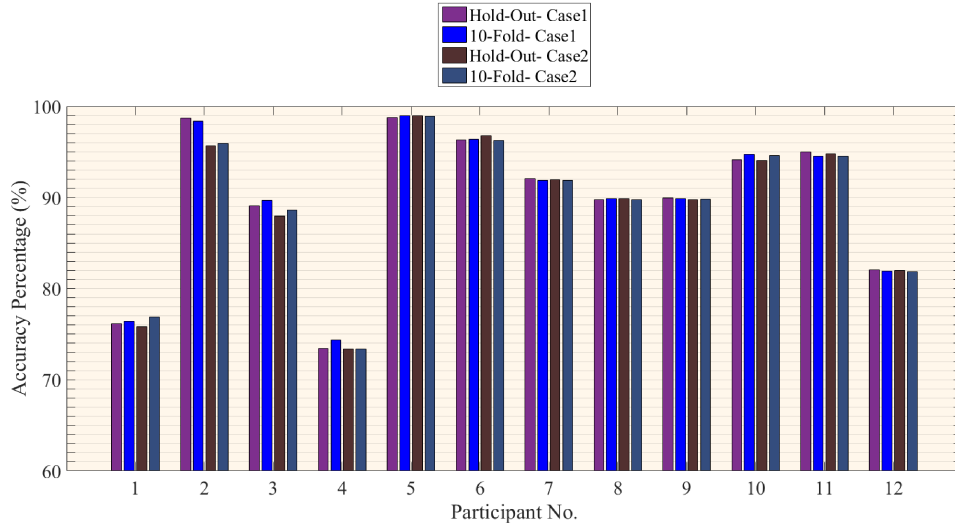


Figure 8: Performance of the best model with Radial Kernel and Cost constant of 100 with both evaluation methods applied to Case 1. Raw dataset and Case 2. Feature extracted dataset, for all of the participants.

400 (False Positive).

Table 4: The actual and predicted labels applied on the whole length dataset. We have 838 False Positives and 146 False Negatives.

	Predicted 0	Predicted 1
Actual 0	2162	838 (FP)
Actual 1	146 (FN)	2854

6. Conclusion and Future Works

In this research article we introduced a novel wearable health monitoring system, MagicSox, that fuses the capabilities of smart textiles with Internet-of-things to detect and communicate gait abnormalities such as drop foot. We provided a detailed technological architecture of MagicSox that can be divided

405

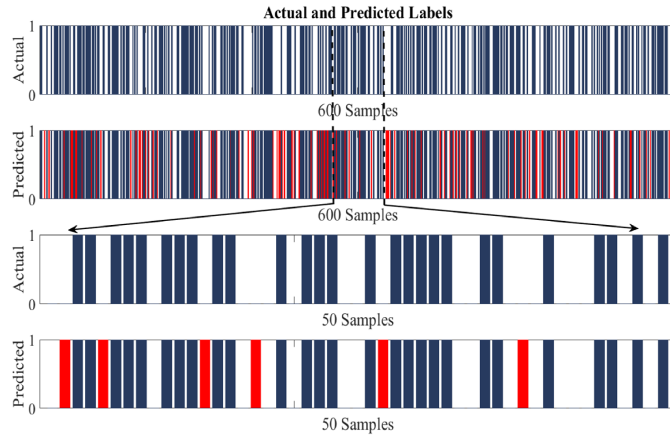


Figure 9: Actual labels and predicted labels of a 600 samples data and the zoomed in picture of 50 samples. White color shows label 0 for normal walking, blue color shows label 1 for drop foot walking and the red color shows the error while the actual label is 0 but the classifier predicts as 1.

into three hardware layers: 1) multi-modal sensors including pressure sensor, 2 flex sensors, and an IMU, 2) an Intel Curie microcontroller with BLE, and 3) an Android smart phone app to collect the data. We pursued experiments on healthy individuals to evaluate the usability and performance of MagicSox. The

410 results showcase that MagicSox is a valuable and reliable tool in quantifying gait abnormalities such as drop foot. Although other studies on the wearable devices for stroke rehabilitation provide 99% accuracy in posture and activity detection [15], the combination of IMU, flex sensors and pressure sensor distinguishes the MagicSox from other devices. The MagicSox can provide more

415 detailed information about the gait cycle, ankle flexion and foot posture. The accelerometer and gyroscope can provide detailed spatial information such as the orientation of the foot, how much swing has been in a gait cycle, how fast or slow the person is walking, and how much they take the foot up in order to complete a gait cycle. The pressure sensor on the heel reveals that if there

420 was a heel strike or not. As discussed earlier, heel strike is necessary for normal walking, and it is not happening in drop foot walking. The flex sensors provide

information about the flexion of the ankle. During a gait cycle, the ankle flexes and stretches and having these flexion and stretches reveals informations about the gait cycle that can be used in rehabilitation to improve the gait cycle of drop foot.

Although our focus in this research was on the quantification of drop foot, MagicSox can also be used for athletes to alert them whenever they have heel strike which can cause serious injuries or pain. It also can be used as an activity tracker to show how many steps a person has taken during the day, or how much distance they have walked. As an immediate next step, we will pursue a pilot study on stroke patients who will wear MagicSox and help us evaluate the system under a clinical setting.

References

- [1] M. E. Hackney, S. Kantorovich, R. Levin, G. M. Earhart, Effects of tango on functional mobility in parkinson's disease: a preliminary study, *Journal of Neurologic Physical Therapy* 31 (4) (2007) 173–179.
- [2] P. Kersten, J. Low, A. Ashburn, S. George, D. McLellan, The unmet needs of young people who have had a stroke: results of a national uk survey, *Disability and rehabilitation* 24 (16) (2002) 860–866.
- [3] F. Lauretani, C. R. Russo, S. Bandinelli, B. Bartali, C. Cavazzini, A. Di Iorio, A. M. Corsi, T. Rantanen, J. M. Guralnik, L. Ferrucci, Age-associated changes in skeletal muscles and their effect on mobility: an operational diagnosis of sarcopenia, *Journal of applied physiology* 95 (5) (2003) 1851–1860.
- [4] J. M. Hausdorff, Gait dynamics, fractals and falls: finding meaning in the stride-to-stride fluctuations of human walking, *Human movement science* 26 (4) (2007) 555–589.
- [5] J. S. Brach, S. Studenski, S. Perera, J. M. VanSwearingen, A. B. Newman,

- 450 Stance time and step width variability have unique contributing impair-
ments in older persons, *Gait & posture* 27 (3) (2008) 431–439.
- [6] J. Rueterbories, E. G. Spaich, B. Larsen, O. K. Andersen, Methods for gait
event detection and analysis in ambulatory systems, *Medical engineering
& physics* 32 (6) (2010) 545–552.
- [7] World heart federation, from, [http://www.world-heart-federation.
455 org/cardiovascular-health/stroke/](http://www.world-heart-federation.org/cardiovascular-health/stroke/).
- [8] Walking abnormalities, by april kahn, medically reviewed by william a
morrison, md on november 30, 2015, from, [http://www.healthline.com/
health/walking-abnormalities/Overview1](http://www.healthline.com/health/walking-abnormalities/Overview1).
- [9] J. D. Stewart, Foot drop: where, why and what to do?, *Practical neurology*
460 8 (3) (2008) 158–169.
- [10] N. B. Alexander, A. Goldberg, Gait disorders: search for multiple causes,
Cleveland Clinic journal of medicine 72 (7) (2005) 586.
- [11] M. Iosa, G. Morone, A. Fusco, M. Bragoni, P. Coiro, M. Multari, V. Ven-
turiero, D. De Angelis, L. Pratesi, S. Paolucci, Seven capital devices for the
465 future of stroke rehabilitation, *Stroke research and treatment* 2012.
- [12] J. M. Winters, Y. Wang, J. M. Winters, Wearable sensors and telerehabili-
tation, *IEEE Engineering in Medicine and Biology Magazine* 22 (3) (2003)
56–65.
- [13] F. Horak, L. King, M. Mancini, Role of body-worn movement monitor tech-
470 nology for balance and gait rehabilitation, *Physical therapy* 95 (3) (2015)
461.
- [14] Q. Wang, W. Chen, A. Timmermans, C. Karachristos, J.-B. Martens,
P. Markopoulos, Smart rehabilitation garment for posture monitoring, in:
2015 37th Annual International Conference of the IEEE Engineering in
475 Medicine and Biology Society (EMBC), IEEE, 2015, pp. 5736–5739.

- [15] S. R. Edgar, T. Swyka, G. Fulk, E. S. Sazonov, Wearable shoe-based device for rehabilitation of stroke patients, in: 2010 Annual International Conference of the IEEE Engineering in Medicine and Biology, IEEE, 2010, pp. 3772–3775.
- 480 [16] A. Mazzoldi, D. De Rossi, F. Lorussi, E. Scilingo, R. Paradiso, Smart textiles for wearable motion capture systems, *AUTEX Research Journal* 2 (4) (2002) 199–203.
- [17] G. Bergmann, H. Kniggenndorf, F. Graichen, A. Rohlmann, Influence of shoes and heel strike on the loading of the hip joint, *Journal of biomechanics* 28 (7) (1995) 817–827.
- 485 [18] J. A. Dickinson, S. D. Cook, T. M. Leinhardt, The measurement of shock waves following heel strike while running, *Journal of biomechanics* 18 (6) (1985) 415–422.
- [19] U. Jørgensen, Body load in heel-strike running: the effect of a firm heel counter, *The American journal of sports medicine* 18 (2) (1990) 177–181.
- 490 [20] L. H. Hamel, *Knowledge discovery with support vector machines*, Vol. 3, John Wiley & Sons, 2011.
- [21] Y. Sun, S. Suppappola, T. A. Wrublewski, Microcontroller-based real-time qrs detection, *Biomedical Instrumentation & Technology* 26 (6) (1992) 477–484.
- 495 [22] S. Suppappola, Y. Sun, Nonlinear transforms of ecg signals for digital qrs detection: a quantitative analysis, *IEEE Transactions on Biomedical Engineering* 41 (4) (1994) 397–400.