

Next-Generation TLC: A Quantitative Platform for Parallel Spotting and Imaging

Alexander A. Boulgakov,[#] Sarah R. Moor,[#] Hyun Hwa Jo,[#] Pedro Metola, Leo A. Joyce, Edward M. Marcotte, Christopher J. Welch,^{*} and Eric V. Anslyn^{*}



Cite This: *J. Org. Chem.* 2020, 85, 9447–9453



Read Online


ACCESS |

Metrics & More

Article Recommendations

Supporting Information

ABSTRACT: A high-throughput screening approach for simultaneous analysis and quantification of the percent conversion of up to 48 reactions has been developed using a thin-layer chromatography (TLC) imaging method. As a test-bed reaction, we monitored 48 thiol conjugate additions to a Meldrum's acid derivative (**1**) in parallel using TLC. The TLC elutions were imaged using a cell phone and a LEGO brick-constructed UV/vis light box. Further, a spotting device was constructed from LEGO bricks that allows simple transfer of the samples from a well-plate to the TLC plate. Using software that was developed to detect “blobs” and report their intensity, we were able to quantitatively determine the extent of completion of the 48 reactions with one analysis.

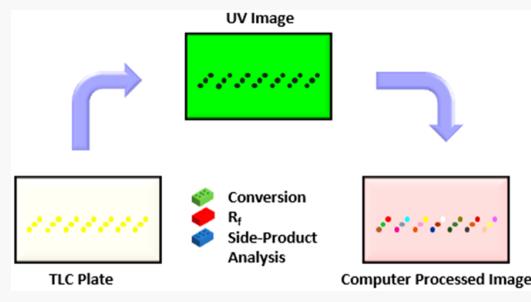

INTRODUCTION

Drug discovery and synthesis optimization rely on modern catalysis to continue advancing. Finding cost-effective routes to both new and existing drugs is a constant area of investigation.¹ High-throughput experimentation (HTE) allows hundreds to thousands of different reaction permutations to be run in a matter of hours and is widely used in the pharmaceutical industry for discovering ligands for receptors, kinases, and enzymes, along with optimizing reaction conditions.² For HTE to succeed, a complementary high-throughput screening (HTS) protocol must be created, otherwise simply by virtue of the multitude of samples, the analysis becomes the bottleneck in the overall discovery process.³ Although many researchers have developed rapid assays for yield determination, the need for more cost-effective assays that do not require specialized or expensive equipment remains.¹ Combining existing separation assays, in this case thin layer chromatography (TLC), with now ubiquitous smartphone capabilities shows promise in addressing these needs.

TLC is one of the most common chromatography techniques used by synthetic chemists to identify compounds in a mixture, determine their purity, and follow the progress of a reaction.⁴ Visualization usually occurs under UV light or by using staining reagents. In the last couple of decades, a number of innovative improvements in TLC have emerged.^{5–7} These have included quantitative analysis via optical scanning, such as is done with commercial TLC scanners.⁸ There have been examples of photometric procedures followed by image processing, as well as using mass spectrometry on the eluted spots.^{9,10} However, these techniques typically put an emphasis on the purity of the samples rather than monitoring reaction

progress and/or determining reaction yield.¹¹ Furthermore, none of the approaches focus on the analysis of multiple reactions simultaneously.

Our group had previously reported a single example of TLC imaging, in this case to prescreen various conditions of an Ir-catalyzed allylation reaction to quantitatively determine their yields.¹² As both the starting material and the product were UV active, we were able to correlate their concentrations to their corresponding spot intensities as observed under UV irradiation. In this report, we extensively expand on this methodology and describe a HTS platform created by combining a TLC multispotter, a light box built from LEGO bricks and spotting device (*vide infra*), an alternating offset arrangement of TLC spots designed to allow for 48 simultaneous analyses, as well as advances in spot-recognition imaging software.

The choice of reaction chemistry to demonstrate the methodology was immaterial to our goals, except that we sought a reaction where conditions could be easily varied. Additionally, although spot-staining for visualization can readily be used in our approach, we sought a reaction where the starting materials and products were UV active. With these considerations in mind, we chose the reaction of a Meldrum's acid derived conjugate acceptor **1** with various nucleophiles


Received: February 11, 2020

Published: June 19, 2020



that act as exchangeable units (E.U.'s, *Scheme 1*).¹³ Compound **1** allows for a coupling of amines and thiols,

Scheme 1. Meldrum's Acid Derived Conjugate Acceptor 1 with Various Thiols or Amines as Nucleophiles^a

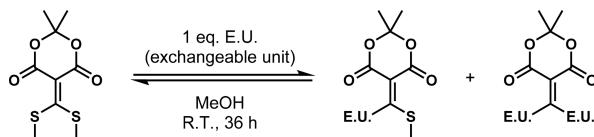

^aE.U. = exchangeable unit.

which can then be decoupled to their starting components using dithiothreitol (DTT). Although this method could provide even more useful data for "cleaner" reactions (i.e., a reaction that gives only one product) to get the yield of the reaction rather than conversion, we chose this exchange reaction to demonstrate the full scope of this technique.

Although **1** has been successfully used for various biological and materials applications, little work has been put into optimizing the thiol or amine exchange reactions. The thiol scrambling is tricky to quantify because it often requires sparging to remove methyl mercaptan. While conventional HPLC analysis is a promising method to monitor this reaction, the sequential elution of each individual sample can make this a tedious, time-consuming method to use for larger scale parallel optimization experiments.¹ TLC, on the other hand, enjoys the relative advantages of low cost, the ability to analyze impure samples, the availability of analyte-specific visualization reagents, and the capability of carrying out multiple simultaneous analyses by spotting multiple samples on each plate and developing several plates in parallel.¹⁴ This parallel analysis capability, along with the fact that TLC imaging has been previously reported,^{8–10} led us to make several improvements such that TLC would be more amenable to HTS. In this paper, we report a method to analyze parallel synthesis procedures in 96-well plates, albeit any plate format is amenable to what is now described.

RESULTS AND DISCUSSION

Our goal was to spot 12 reactions at a time from a 96-well plate (8×12 strips) wherein the reactions of *Scheme 1* were performed using amines and thiols as the exchangeable units (E.U.'s, *Supplementary Table 1*). Although 96 reactions could have been screened, the methodology now described was most successful with only half the plate, i.e., 48 reactions. The amount of sample delivered and the spreading during spotting can affect both resolution and smearing of the eluted spots. Thus, as any practitioner of TLC knows, the spotting of the plate is crucial to success. As many of the reactions of compound **1** with amines or thiols give multiple products (monosubstituted, disubstituted, and polymerized), failing to properly control amounts dispensed would result in eluted product spots that are too broad and hence show extensive overlap with spots from other lanes. For this reason, it was vital to have a TLC spotter that would dispense small initial volumes ($<1 \mu\text{L}$), yet sturdy enough to place all 12 spotters flat on the plate.^{15,16} While we initially created a hand-held 3D-printed spotter that accommodated 12 steel needles, the operator needed to carefully touch all 12 needles at once to the silica on the plate and press lightly so that the needles are not

plugged with silica. The fact that the spot intensity across the 12 needles was dependent upon careful control by the operator prompted us to devise a less variable spotting method.

We turned to the use of a LEGO spotter, shown in *Figure 1*, as a design for those laboratories that do not have access to a

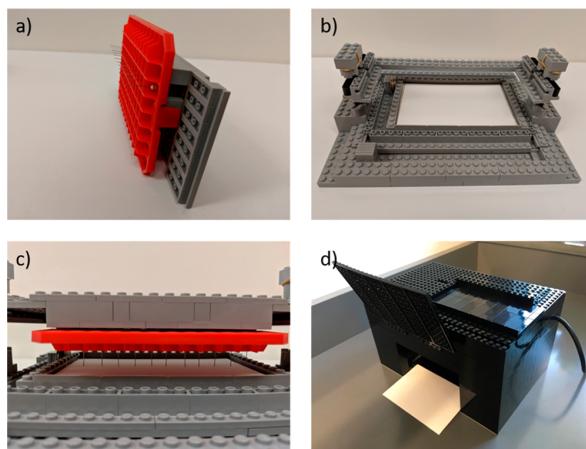


Figure 1. (a) LEGO holder to be loaded with blunted syringe needles, (b) TLC carriage, (c) LEGO spotter/holder placed on carriage, (d) LEGO black box with UV lamp in back.

3D-printer, and operators with slightly shaky hands. This easy to assemble, user-friendly setup yields the capability to perform spotting in a reproducible, staggered manner (to obtain four rows of 12 spots, i.e., 48 spots in total) and the added potential for customization. The first part of the spotter is a holder where the 12 blunt-nosed needles are arranged linearly in regular intervals using a mounting-piece created from a pipet tip box (*Figure 1a*). The second piece is the base of the spotter (carriage), which consists of a cavity to hold the TLC plate on two sliding panels with two sets of three removable spacers (*Figure 1b*). Once the carriage is loaded with the holder, the four columns on the sides allow for vertical movement perpendicular to the plane of the TLC plate that provides the spotting (*Figure 1c*). The holder can be detached from the carriage for loading of the samples from an installed 96-well plate and then reassembled to allow for spotting of an installed TLC plate. This latter operation must be conducted using both hands and adjusting the timing of contact between tips and plate to ensure uniform and efficient spotting. Importantly, because of the controlled sliding of the holder up and down along the four posts, the needles all touch simultaneously, reducing operator error. Once the first row of 12 samples are spotted, the two sets of spacers come into action: removing one spacer in each set allows two sliders to move (one along the X axis and the other along the Y axis) before performing the next round of 12 sample spotting, which thereby occurs slightly to the right and above the initial row of 12 spots. The movement of the sliders is akin to playing hop-scotch, where one jumps to the right and then forward, thus moving diagonally a controlled distance. This operation is repeated three times for the total of 48 samples before the TLC is developed and analyzed in a LEGO black box (*Figure 1d*). After each spotting of the TLC plate, the needles are emptied by touching filter paper and a wash with acetone to remove excess solution so as to not contaminate the next set of 12 spots.

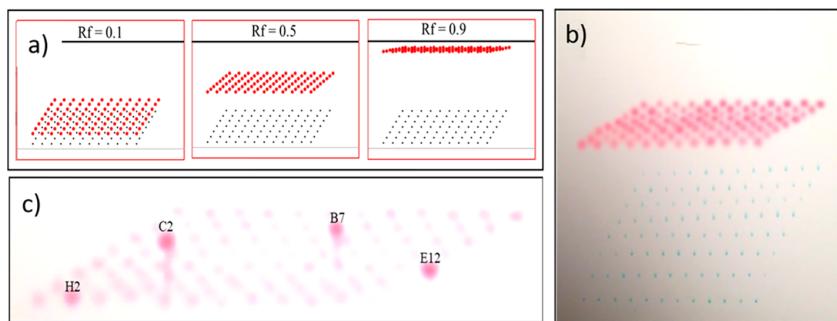


Figure 2. Modeling and initial studies using dyes from microplates spotted on TLC plates using a staggered spotting approach. (a) Excel modeling showing “sweet spot” of R_f ~0.5 for most effective visualization. (b) Elution of spots from a 96-well plate containing samples of methylene blue (R_f ~0) and methyl red (R_f ~0.6) using 95% ethanol/water. (c) Analysis of plate containing four wells spiked with additional methyl red allows easy determination of the “address” of the hits.

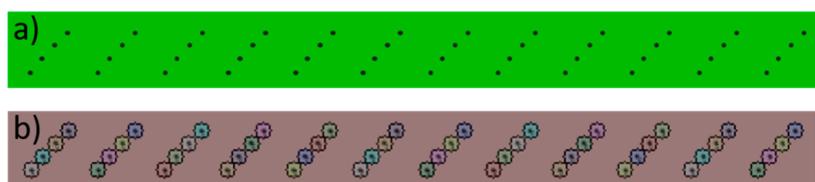


Figure 3. (a) Computer-generated model TLC plate. (b) Model TLC plate post software analysis.

In a previous report, we described the use of a LEGO black box as a simple and inexpensive alternative to a fluorescence 96-well plate reader.¹⁴ Herein, a variant was used for visualization of the TLC plates with a common UV lamp, with data recording via cell phone photography, followed by the use of chromaticity/luminosity for data analysis (vide infra). The LEGO loading stage was modified to hold TLC plates (Figure 1d) rather than 96-well plates. This simple modification demonstrates one strength of using LEGO bricks for the construction of instruments rather than 3D-printing. The device can be easily reconfigured for numerous purposes without the generation of a new CAD-file and the time taken for printing. This is further exemplified with the above-described TLC spotter. Albeit some time was taken to imagine the operations and then optimize the apparatus, creating such a device with moving parts out of materials other than LEGO bricks would have been significantly more challenging and more expensive to repair or replace when needed.

For analysis of reactions in a standard 96-well plate, we explored the direct spotting of rows of samples (0.9 mm well to well spacing) onto a standard 20 × 20 cm TLC plate. Only a single complete row of 12 spots can fit onto a single TLC plate, and while strategies for interleaving additional rows of spots along the origin line are possible, we found the resulting developed TLC plates to be highly congested and difficult to interpret. Thus, we investigated an alternative spotting strategy in which spots from rows A, B, C, D, etc. are offset in both the horizontal and vertical direction (Figure 2). Interestingly, modeling using 96 spots shows this technique to produce a profile of product spots that takes the form of a skewed 8 × 12 grid when the R_f of the eluted compound of interest are all the same and between about 0.3 and 0.6 (Figure 2a), with higher or lower R_f values producing congested images that are difficult to interpret. Demonstration of the approach is shown in Figure 2b, where a 96-well microplate containing a mixture of two dyes: methylene blue (R_f ~0) and methyl red (R_f ~0.6) is

eluted using 95% ethanol/water. The red dye elutes up the plate while the blue dye stays at the baseline. The analysis of a TLC plate containing four wells with higher levels of methyl red affords a straightforward identification of the “address” of these spots (Figure 2c).

Having demonstrated that 12 reactions can be spotted in a row, and the next 12, and so forth, in a diagonally staggered manner to minimize the interference from the spots when the plate is developed, we turned our attention to photographic plate imaging. To start, a computer-generated image of identical noneluted spots was created to demonstrate the accuracy of the software (Figure 3a).

Forty-eight spots were used to emulate reaction spots. These spots were then analyzed by the software with an average deviation of 1.6 (Figure 3b). However, as these spots were computer generated and TLCs are subject to human error, we expected that real plates analysis would not be so accurate. These promising results prompted us to analyze complex reaction mixtures.

In our preliminary report of TLC quantitative imaging for determining reaction yield, we generated a calibration curve for the spot intensity of the product.¹² In the current study, we created a calibration curve to demonstrate how concentration can be detected and quantified using our image analysis program (vide infra). Nine samples of varying concentrations of **1**, ranging from 20 to 200 μ M, were spotted on a plate and eluted with 3:1 hexanes/ethyl acetate (v/v). Figure 4a shows a photo taken with an iPhone using the black box constructed of LEGO bricks under UV radiation (Figure 1).¹⁴ The solvent system was devised such that the spots have an R_f value of 0.5 (vide supra), and all spots on the plate were automatically detected. The intensity of each spot was then measured using an algorithm that we developed (Figure 4b, details below). By plotting the measured intensity versus concentrations of **1**, a calibration curve was generated (Figure 4c). Here, 200 μ M of **1** corresponds to 100% of **1** remaining in a reaction of any well

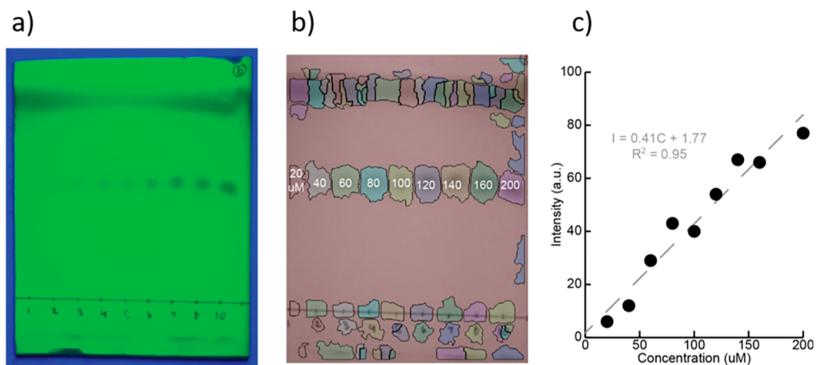


Figure 4. (a) Calibration plate is spotted with known concentrations of analyte **1** and eluted. (b) Eluted spots are segmented and their intensities are quantified. Loading concentration of each reaction is indicated in μM . (c) Linear calibration curve ($R^2 = 0.95$) generated from varying concentrations of **1**.

in the plate, while lower spot intensities are used to estimate the percent completion of the reaction. This demonstrates the software's ability to quantify different spot concentrations.

The conjugate addition reaction with **1** was performed in methanol with various amines and thiols (Supplementary Table S1) in 48 wells of a 96-well plate for 36 h (initial concentration of **1** = 0.25 mM). We used 48 reactions rather than 96 because the overlap of the spots was too severe when 96 samples of varying R_f values for the products were spotted. All the reactions were performed in a 96 deep-well plate and were then spotted on to the silica plate using the in-house LEGO spotter and the experimental details given above associated with our discussion of Figure 1a. Using the spotting configuration discussed above, the 48 reactions were eluted in 3:1 hexanes/ethyl acetate (v/v). The eluted spots were then analyzed using our processing script to get spot intensities for each well, as now described.

TLC plate images were analyzed in a semiautomated fashion to measure spot intensities for each analyte. These intensities were then used to determine the reaction yields based on the average control starting **1** spot intensity as described below (Supplementary Table S1). But first, we describe the image processing steps used. While the ultimate plan is for an interactive smart-phone app to semiautomatically analyze the TLC plates with assistance from the user, for now we have developed a desktop GUI that accomplishes this task. Our code is available on Github at <https://github.com/marcottelab/appaloosa>, with a sample image and a walkthrough manual to get started. It primarily utilizes Scikit-Image for its image morphology routines.¹⁵

We begin the analysis of each image by cropping it to the plate and converting it to grayscale, so that spots are dark objects on a light background. This grayscale image is then median corrected to standardize brightness across the plate and remove any bias due to positioning of the UV/vis lamp on the LEGO box. To identify reaction spots, we perform one round of waterfall segmentation to isolate areas containing spots from the background, and then to this isolated foreground we apply one round of watershed segmentation to subdivide it into spots corresponding to individual reactions.^{17,18} Both waterfall and watershed segmentations treat pixel values in an image as a terrain, as in a grassy knoll. In this analogy, each dark spot forms a depression—or drainage ditch—that are isolated from their neighbors along ridge lines analogous to dividing ranges in geography, or boundaries of

counties/cities on a map. The waterfall algorithm is more wary of oversegmentation and is hence applied before the more sensitive watershed algorithm. If we were to apply a watershed segmentation immediately, without the initial waterfall round, we would be likely to “identify” many spurious “spots” in the background. Hence the need for a two-round approach.

Although we have chosen the default parameters used by the second segmentation step to work well with the majority of TLC plates, sometimes the resulting segmentation is not sufficiently fine-grained to separate spots that are very faint or blur together. In such cases, we rely on the user to direct the software via the interactive GUI. The user can direct the software to attempt a finer-grained subdivision of a particular spot, or to subdivide spots by hand. We provide examples of each operation in our Github walkthrough. Note that such manual subdivisions can be applied iteratively until a satisfactory result is obtained, making the interactive aspect of our software very powerful. Finally, it is possible to cast all identified spots into circles. This is accomplished by identifying potential circular features of each spot with a Laplacian of Gaussian¹⁹ and then from these choosing the circular feature (i.e., circle) that maximizes the average intensity per unit area as captured by the circle. Figure 5 shows an example eluted TLC plate with a final spot segmentation, including both automatically and manually segmented spots, all finally converted into circles around the spot. Another useful functionality in the GUI is the ability for the user to manually define the baselines for reactions, as well as the solvent front. Once this is done, it is possible to assign spots to different baselines and from this their R_f values can be calculated. Again, our walkthrough provides an example.

Once the spots are segmented, we measure their intensity against the background as a proxy for analyte amount. We take the sum of pixel values within a segmented spot as its raw intensity. To obtain background intensity, we scale the spot's bounding box to twice its area, and then take the median of pixel intensities within the box that are outside of any other adjacent segmented spots. We correct for the background by subtracting from the raw intensity the background intensity multiplied by the area of the spot (across which pixels were summed).

Once all the software had been developed, we turned to actual TLC analysis using **1** and various E.U.'s (Supplementary Table S1). We assigned a subset of the wells as control reactions (#5, #18, #31, and #44, Supplementary Table S1) to

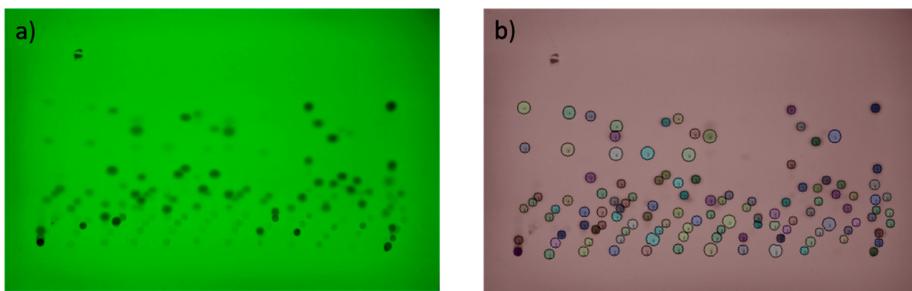


Figure 5. (a) Eluted TLC plate spotted with 48 reactions. (b) Sci-kit analyzed image of the eluted TLC plate.

Table 1. Percent Composition of 1 Obtained Using NMR and LC/MS Spectra^a

	TLC spot intensity (%)	TLC yield (%)	assay yield (%)	% error
control	70			
1,4-phenylenediamine	0	100	100	0
1-dodecanethiol	55	21	12	9
2-mercaptopropanoic acid	72	-3	0	2
1,4-butanedithiol	86	-23	10	33
3,6-dioxa-1,8-octane-dithiol	57	19	0	22
<i>p</i> -xylylenediamine	0	100	100	0
1-decanethiol	67	4	20	16
4-methoxybenzylamine	0	100	96	4
dodecylamine	0	100	100	0
<i>N</i> -benzylmethylamine	0	100	94*	6
avg error				9

^aAll yields were determined via NMR except those marked by an “*” to denote the yield were determined via LC/MS.

have no E.U.’s. These wells were chosen to give a distribution of spots across the plate to account for differences in lamp light. Thus, the resulting spots would be solely due to 1 which has a $R_f = 0.38$. Using the GUI interference, we can manually extrapolate the solvent front position to calculate R_f values. By marking the starting position of each baseline, we can assign eluted spots to the original baseline positions (i.e., one of four), as well as classify whether they are unreacted analyte (i.e., whether they lie on a corresponding $R_f = 0.38$ lines). To calculate the extent of reaction and compare to the average intensity of the control reactions, and calculate the amount of reacted vs unreacted starting material (Supplementary Table S2). This is done for all 48 spots. From the measured spot intensities, the concentration of 1 remaining in the reaction was calculated using the starting intensity of the 1 control samples, wells #5, #18, #31 and #44, which had an average intensity of 71. The concentration data can then be converted to percent of 1 remaining after 36 h, which allows us to estimate conversion of the reaction. Of course, as done in our previous report, the calibration curve Figure 3 can alternatively be used to quantitate remaining starting material.¹²

In order to test the accuracy of the data collected, NMR and LC/MS was performed on 10 randomly selected reactions to estimate percent starting material remaining (Table 1). When the two values were compared, the average absolute difference between starting material as detected by LC/MS and TLC was 9%. Although the average error is quite low, the error associated with some reactions was significantly higher than this average. Looking closer, the reactions can be classified into two rather distinct groups: the first, with 7 out of 10 reactions, which did not suffer spot overlap and hence were accurately quantified with an average absolute error of 3%; and the second, with the remaining 3 out of 10 reactions, which

suffered spot overlap and hence were quantified with an average error of 25% (which is still rather informative in many cases). The larger errors in the second group can be attributed to overlap between adjacent spots, in some cases when they were initially spotted and others after the plate was run. For example, 1,4-butanedithiol (spot 4, Supplementary Figure S1), has significant overlap with its adjacent spot. Such errors can be remedied with careful spotting or if cleaner reactions are screened. In addition, due to the unique shape of our TLC plate, an improvised TLC chamber was used which results in some slight curving of the TLC spots as the plate was eluted. Thus, the TLC method gave an error of under 10% in determining extent of reaction of 1 with the various E.U.’s.

Having found success with a parallel analysis of 48 reactions via TLC for HTS purposes, it is important to discuss limitations and complications. First, we are relying on a UV lamp, and the kind of lamp, how long one waits to take the picture after turning on the lamp, all affect the images. Second, the camera used, or the box (i.e., the darkness of the surroundings) will influence the result as well. Any overlap between spots will affect adjacent spots, making it imperative to have the spots properly staggered and ensuring the TLC runs straight. Lastly, consistency in spot size and between the analysis and calibration plates is critical, and the LEGO spotter nicely assists in this regard. However, as long as one is consistent with all the experimental procedures and settings, our overall TLC methodology gives reliable data that can be used to quantitate the yield and/or percent completion of numerous reactions simultaneously. While this manuscript focused on optical detection of TLC spots, an analogous approach may prove useful for DESI or MALDI mass spectroscopy imaging of TLC plates.

■ SUMMARY

TLC is the most common bench-side quick analytical test for examining the progress of chemical reactions. While multiple TLC spots along a single line is common for qualitatively analyzing various samples collected from flash-chromatography, such spotting has not been previously converted to a parallel method for reaction screening and yield quantitation. The overall approach described herein for analyzing 1/2 of a 96-well plate is simple, fast, and user friendly. It involves a 12-needle dispensing device constructed from LEGO bricks, a LEGO black box for photography, and an extensive software suite available on Github. We anticipate that this work will facilitate reaction discovery and optimization as well as inspire further improvements on this classic and simple analytical method.

■ EXPERIMENTAL SECTION

Conversion Validation. Stock solutions (40 mM, 0.02 mmol) of each compound (Supplementary Table S1) and compound 1 (40 mM, 0.02 mmol) were made in CD₃OD. From the stock solutions of each compound and compound 1, 500 μ L of each were mixed in a 1:1 ratio in vials and left to sit for 48 h. After 48 h, 1 mL of a 20 mM stock solution of 1,3,5-trimethoxybenzene was added in a 1:1 mixture with the reaction mixtures. The samples were then analyzed via NMR. For N-benzylmethylamine, the reaction mixtures along with the control reaction were diluted with CD₃OD and analyzed via LC/MS.

■ ASSOCIATED CONTENT

Supporting Information

The Supporting Information is available free of charge at <https://pubs.acs.org/doi/10.1021/acs.joc.0c00349>.

General procedure, synthesis, and characterization of compound 1, TLC analysis, ¹H NMR and LC/MS spectral data for reaction 1 yield analysis, Appaloosa Thin Layer Chromatography Wizard User Manual (PDF)

■ AUTHOR INFORMATION

Corresponding Authors

Christopher J. Welch – Department of Process Research and Development, Merck & Co., Inc., Rahway, New Jersey 07065, United States;  orcid.org/0000-0002-8899-4470; Email: christopher@welchinnovation.com

Eric V. Anslyn – Center for Systems and Synthetic Biology/ Institute for Cellular and Molecular Biology, Department of Molecular Biosciences, The University of Texas at Austin, Austin, Texas 78712, United States; Email: anslyn@austin.utexas.edu

Authors

Alexander A. Boulgakov – Center for Systems and Synthetic Biology/ Institute for Cellular and Molecular Biology, Department of Molecular Biosciences, The University of Texas at Austin, Austin, Texas 78712, United States

Sarah R. Moor – Department of Chemistry, The University of Texas at Austin, Austin, Texas 78712, United States;  orcid.org/0000-0001-5579-407X

Hyun Hwa Jo – Department of Chemistry, The University of Texas at Austin, Austin, Texas 78712, United States

Pedro Metola – Department of Chemistry, The University of Texas at Austin, Austin, Texas 78712, United States

Leo A. Joyce – Department of Process Research and Development, Merck & Co., Inc., Rahway, New Jersey 07065, United States;  orcid.org/0000-0002-8649-4894

Edward M. Marcotte – Center for Systems and Synthetic Biology/ Institute for Cellular and Molecular Biology, Department of Molecular Biosciences, The University of Texas at Austin, Austin, Texas 78712, United States

Complete contact information is available at: <https://pubs.acs.org/10.1021/acs.joc.0c00349>

Author Contributions

[#]A.A.B., S.R.M., and H.H.J. contributed equally.

Notes

The authors declare no competing financial interest.

■ ACKNOWLEDGMENTS

We gratefully acknowledge support from the following funding sources: National Science Foundation to A.A.B. (DGE-1610403) and an NSF GOALI (1665040), the National Institutes of Health (1 S10 OD021508-01), the Howard Hughes Medical Institute (GT10481), and the Welch Regents Chair to E.V.A. (F-0046). E.M.M. acknowledges funding from the NSF, NIH, and Welch Foundation (F-1515). We acknowledge Sarah Moor for her contributions to the cover art.

■ REFERENCES

- (1) Herrera, B. T.; Pilicer, S. L.; Anslyn, E. V.; Joyce, L. A.; Wolf, C. Optical Analysis of Reaction Yield and Enantiomeric Excess: A New Paradigm Ready for Prime Time. *J. Am. Chem. Soc.* **2018**, *140* (33), 10385–10401.
- (2) Krska, S. W.; DiRocco, D. A.; Dreher, S. D.; Shevlin, M. The Evolution of Chemical High-Throughput Experimentation To Address Challenging Problems in Pharmaceutical Synthesis. *Acc. Chem. Res.* **2017**, *50* (12), 2976–2985.
- (3) Mayr, L. M.; Fuerst, P. The Future of High-Throughput Screening. *J. Biomol. Screening* **2008**, *13*, 443.
- (4) Gordon, A. J.; Ford, R. A. *The Chemist's Companion: A Handbook of Practical Data, Techniques, and References*, 1st ed.; Wiley: New York, 1972.
- (5) Attimaran, M.; Ahmed, K. K. M.; Aldhubaib, B. E.; Harsha, S. High-Performance Thin Layer Chromatography: A Powerful Analytical Technique in Pharmaceutical Drug Discovery. *Pharm. Methods* **2011**, *2* (2), 71–75.
- (6) Fichou, D.; Morlock, G. E. Open-Source-Based 3D Printing of Thin Silica Gel Layers in Planar Chromatography. *Anal. Chem.* **2017**, *89* (3), 2116–2122.
- (7) Morlock, G. E.; Oellig, C.; Bezuidenhout, L. W.; Brett, M. J.; Schwack, W. Miniaturized Planar Chromatography Using Office Peripherals. *Anal. Chem.* **2010**, *82* (7), 2940–2946.
- (8) Stroka, J.; Spangenberg, B.; Anklam, E. New Approaches in TLC-Densitometry. *J. Liq. Chromatogr. Relat. Technol.* **2002**, *25* (10–11), 1497–1513.
- (9) Lancaster, M.; Goodall, D. M.; Bergström, E. T.; McCrossen, S.; Myers, P. Real-Time Image Acquisition for Absorbance Detection and Quantification in Thin-Layer Chromatography. *Anal. Chem.* **2006**, *78* (3), 905–911.
- (10) Morlock, G.; Schwack, W. Planar Chromatography Coupled to Mass Spectrometry. *TrAC, Trends Anal. Chem.* **2010**, *29*, 1157–1171.
- (11) Ferenczi-Fodor, K.; Végh, Z.; Renger, B. Thin-Layer Chromatography in Testing the Purity of Pharmaceuticals. *TrAC, Trends Anal. Chem.* **2006**, *25*, 778–789.
- (12) Jo, H. H.; Gao, X.; You, L.; Anslyn, E. V.; Krische, M. J. Application of a High-Throughput Enantiomeric Excess Optical Assay Involving a Dynamic Covalent Assembly: Parallel Asymmetric Allylation and Ee Sensing of Homoallylic Alcohols. *Chem. Sci.* **2015**, *6* (12), 6747–6753.

(13) Diehl, K. L.; Kolesnichenko, I. V.; Robotham, S. A.; Bachman, J. L.; Zhong, Y.; Brodbelt, J. S.; Anslyn, E. V. Click and Chemically Triggered Declick Reactions through Reversible Amine and Thiol Coupling via a Conjugate Acceptor. *Nat. Chem.* **2016**, *8* (10), 968–973.

(14) Poole, C. F.; Poole, S. K. Instrumental Thin-Layer Chromatography. *Anal. Chem.* **1994**, *66* (1), 27A–37A.

(15) Thoden, J. Spotter for Use in Thin Layer Chromatography and Method of Forming Drops Therewith. US3843053A, 1974-10-22.

(16) Musil, F.; Fosslien, E. An Automatic Eight-Channel Spot Applicator for Thin-Layer Chromatography. *J. Chromatogr. A* **1970**, *47*, 116–118.

(17) Terol-Villalobos, I. R.; Mendiola-Santibañez, J. D. Transformations with Reconstruction Criteria: Image Segmentation and Filtering. In *Mathematical Morphology: 40 Years On*; Ronse, C., Najman, L., Decencière, E., Eds.; Computational Imaging and Vision, Springer Netherlands: Dordrecht, 2005; pp 75–84. DOI: 10.1007/1-4020-3443-1_8.

(18) Meyer, K. H. Fritz Ullmann 1875–1939. *Helv. Chim. Acta* **1940**, *23* (1), 93–100.

(19) van der Walt, S.; Schönberger, J. L.; Nunez-Iglesias, J.; Boulogne, F.; Warner, J. D.; Yager, N.; Gouillart, E.; Yu, T. Scikit-Image: Image Processing in Python. *PeerJ* **2014**, *2*, No. e453.