

PAPER

Flexible, high-resolution thin-film electrodes for human and animal neural research

To cite this article: Chia-Han Chiang *et al* 2021 *J. Neural Eng.* **18** 045009

View the [article online](#) for updates and enhancements.

**PAPER**

RECEIVED
14 February 2021

REVISED
5 May 2021

ACCEPTED FOR PUBLICATION
19 May 2021

PUBLISHED
17 June 2021

Flexible, high-resolution thin-film electrodes for human and animal neural research

Chia-Han Chiang^{1,15} , Charles Wang^{1,15} , Katrina Barth¹ , Shervin Rahimpour² , Michael Trumpis¹ , Suseendrakumar Duraivel¹ , Iakov Rachinskiy¹ , Agrita Dubey³ , Katie E Wingel³, Megan Wong¹, Nicholas S Witham^{4,5}, Thomas Odell⁵, Virginia Woods¹, Brinnae Bent¹ , Werner Doyle⁶, Daniel Friedman⁷ , Eckardt Bihler⁸, Christopher F Reiche⁴ , Derek G Southwell² , Michael M Haglund², Allan H Friedman², Shivanand P Lad², Sasha Devore⁷ , Orrin Devinsky^{6,7,9} , Florian Solzbacher^{4,5,10} , Bijan Pesaran^{3,7} , Gregory Cogan^{2,12,13,14,*} and Jonathan Viventi^{1,2,11,14,*}

¹ Department of Biomedical Engineering, Duke University, Durham, NC, United States of America

² Department of Neurosurgery, Duke School of Medicine, Durham, NC, United States of America

³ Center for Neural Science, New York University, NY, NY, United States of America

⁴ Department of Electrical and Computer Engineering, University of Utah, Salt Lake City, UT, United States of America

⁵ Department of Biomedical Engineering, University of Utah, Salt Lake City, UT, United States of America

⁶ Department of Neurosurgery, NYU Langone Medical Center, New York City, NY, United States of America

⁷ Department of Neurology, NYU Grossman School of Medicine, NY, NY, United States of America

⁸ DYCONEX AG, Bassersdorf, Switzerland

⁹ Comprehensive Epilepsy Center, NYU Langone Health, NY, NY, United States of America

¹⁰ Department of Materials Science & Engineering, University of Utah, Salt Lake City, UT, United States of America

¹¹ Department of Neurobiology, Duke School of Medicine, Durham, NC, United States of America

¹² Department of Psychology and Neuroscience, Duke University, Durham, NC, United States of America

¹³ Center for Cognitive Neuroscience, Duke University, Durham, NC, United States of America

¹⁴ Duke Comprehensive Epilepsy Center, Duke School of Medicine, Durham, NC, United States of America

¹⁵ These authors contributed equally to this work.

* Authors to whom any correspondence should be addressed.

E-mail: j.viventi@duke.edu and gregory.cogan@duke.edu

Keywords: intraoperative, ECoG, electrode, iEEG, LCP, Brain Machine Interface (BMI), Neural Interface

Supplementary material for this article is available [online](#)

Abstract

Objective. Brain functions such as perception, motor control, learning, and memory arise from the coordinated activity of neuronal assemblies distributed across multiple brain regions. While major progress has been made in understanding the function of individual neurons, circuit interactions remain poorly understood. A fundamental obstacle to deciphering circuit interactions is the limited availability of research tools to observe and manipulate the activity of large, distributed neuronal populations in humans. Here we describe the development, validation, and dissemination of flexible, high-resolution, thin-film (TF) electrodes for recording neural activity in animals and humans. **Approach.** We leveraged standard flexible printed-circuit manufacturing processes to build high-resolution TF electrode arrays. We used biocompatible materials to form the substrate (liquid crystal polymer; LCP), metals (Au, PtIr, and Pd), molding (medical-grade silicone), and 3D-printed housing (nylon). We designed a custom, miniaturized, digitizing headstage to reduce the number of cables required to connect to the acquisition system and reduce the distance between the electrodes and the amplifiers. A custom mechanical system enabled the electrodes and headstages to be pre-assembled prior to sterilization, minimizing the setup time required in the operating room. PtIr electrode coatings lowered impedance and enabled stimulation. High-volume, commercial manufacturing enables cost-effective production of LCP-TF electrodes in large quantities. **Main Results.** Our LCP-TF arrays achieve 25× higher electrode density, 20× higher channel count, and 11× reduced stiffness than conventional clinical electrodes. We validated our LCP-TF electrodes in multiple human intraoperative recording sessions and have disseminated this technology to >10 research groups. Using these arrays, we have

observed high-frequency neural activity with sub-millimeter resolution. *Significance.* Our LCP-TF electrodes will advance human neuroscience research and improve clinical care by enabling broad access to transformative, high-resolution electrode arrays.

1. Introduction

The brain is a complex control center that processes and responds to sensory inputs and coordinates a range of functions from physiological (muscles and organs) to psychological (mood and thoughts). These operations involve organized activity of large neuronal populations across multiple brain regions. To record brain activity with large spatial coverage, intracranial electroencephalography (iEEG), or electrocorticography (ECoG), is commonly used. ECoG utilizes a soft and flexible array of metal disc electrodes to sense neural activity (local field potential, LFP) from the surface of the cortex. Although ECoG is mainly used to plan epilepsy surgeries, it can reliably record signals over years after implantation [1], which makes it also a promising interface for chronically implantable neural prostheses [2].


Advances in microfabrication techniques have created electrode arrays with sub-millimeter resolution [3–6]. These micro-fabricated ECoG arrays (micro-ECoG, or μ ECoG) can measure rich microscale neural-dynamics that were previously undetectable by coarsely sampled (centimeter scale) clinical grids (CG). For example, fine-scale spatial temporal patterns emerge in an induced seizure model when sampled with sub-mm resolution [7]. Furthermore, with increases in spatial resolution, action potentials can be recorded from the cortical surface [8]. Therefore, reducing electrode-site size and increasing electrode density enables sensing of signals from the cortex that are undetectable with standard CGs.

For clinical applications in epilepsy patients, high density electrodes can improve diagnostic efficacy by better defining the epileptogenic cortex [9]. Standard CGs, which contain macroelectrodes alone (2.3 mm diameter, 10 mm spacing), sparsely sample epileptiform tissue and lack the signal resolution necessary to resolve focal neuronal sources. Microelectrode arrays for seizure diagnostics offer higher spatial resolution [10, 11], improved seizure detection rates [12], and may identify precursors that predict clinical seizures [12, 13]. For instance, microscale electrode arrays can better detect high-frequency broadband neural activity which has been shown to have high correlation with multi-unit spiking activity [14], high-frequency oscillations (HFOs) [15–17] and microseizures [13, 18, 19] that are missed or poorly sampled with CG electrodes. Microseizures can be detected more than one minute earlier than the signals recorded with typical CGs [13]. Enabling broad access to microelectrodes would allow the measurement

of microseizures to become part of routine clinical care and could improve seizure warning systems [20, 21].

The potential for microscale signals to better inform seizure diagnostics, as well as research on cognition [22] and brain-machine interfaces [5, 23–26], has motivated several electrode manufacturers to integrate protruding microwires into clinical macroelectrode grids. Several of these devices have FDA approval but technical challenges limit their widespread adoption. Commercial microwire grids have very high and varying impedances (<100 k Ω to 6–8 M Ω), owing to their non-uniform exposure from the insulating substrate. Additionally, their 'sharp, ragged' metal edges can damage the brain [27]. Recording from microelectrodes with clinical data acquisition (DAQ) systems can distort signals because microelectrodes have far higher impedances than macroelectrodes [28] and require amplifiers with higher input impedances to produce reliable, low noise recordings with minimal cross-talk [29]. Finally, microwire hybrid grids typically only have a small number of microwire electrodes (~16) and limited coverage due to limitations in the clinical connector design [13, 30, 31]. Therefore, although microelectrodes have been introduced into clinical applications, their integration remains limited.

To meet the need for high-resolution neural interfaces that could enhance scientific discovery and advance clinical therapies, we have developed, extensively tested, and successfully recorded from novel electrode arrays based on thin-film (TF) technology using liquid crystal polymer (LCP) manufactured by our medical device manufacturing partner Dyconex AG. In previous studies, we developed a 61ch array and tested its chronic reliability for over 1 year in rats [32]. We have also developed a 244ch array for use in non-human primates (NHP), with the capability to simultaneously record from individually movable, penetrating microelectrodes [33]. In this paper, we demonstrate improvements on these prior results by translating LCP-TF electrodes to human intraoperative research, including electroplating electrode contacts with platinum iridium (PtIr) to enable stimulation. We provide demonstrations of intraoperative recordings that highlight the focal information that can be captured with LCP-TF electrodes that may be missed with CGs. We also developed a complete electrical and mechanical recording setup to facilitate efficient intraoperative research and rapid dissemination of LCP-TF electrodes to interested researchers.

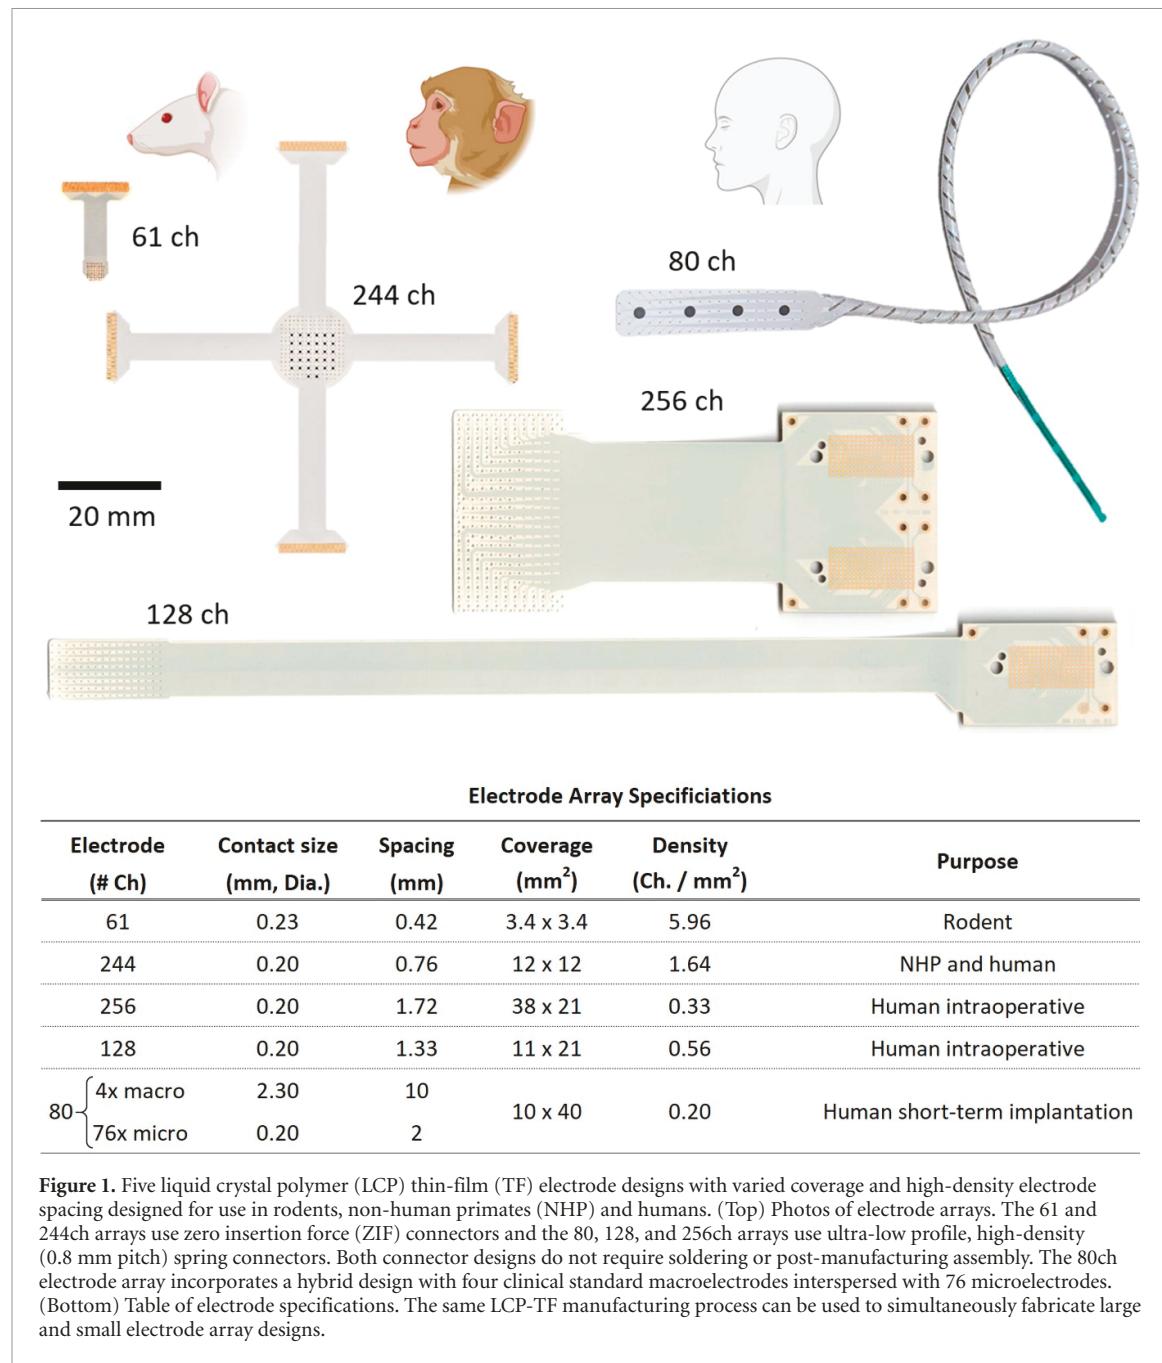

Our advances in electrode manufacturing, design, and implementation will enable high-channel count, micro-scale human neuroscience research.

in figure 1 were fabricated with our medical device manufacturing partner, Dyconex, AG (CH).

2. Material and methods

2.1. Electrode

We have designed five LCP-TF electrodes for different applications (figure 1) ranging from rodents to humans. High-resolution electrodes typically require expensive semiconductor micro-fabrication techniques in a cleanroom environment, which makes large scale production and wide dissemination challenging. We leveraged flexible printed circuit (FPC) technology to inexpensively manufacture a large quantity of LCP-TF electrodes. All electrodes shown

2.1.1. LCP material

Fabricating electrodes using LCP offers many advantages. LCP is long-lasting, with water permeability $\sim 25 \times$ lower than commonly used FPC materials such as polyimide [34], which dramatically extends implanted array reliability and lifetime. LCP is also a self-adhering thermoplastic material, which requires no additional adhesives or glues when combining multiple sheets. Accelerated aging studies project that the devices would maintain their electrical performance for at least 5 years when implanted [32]. By contrast, polyimide electrode arrays rely on interlayer adhesion and can delaminate in < 1 year [32].

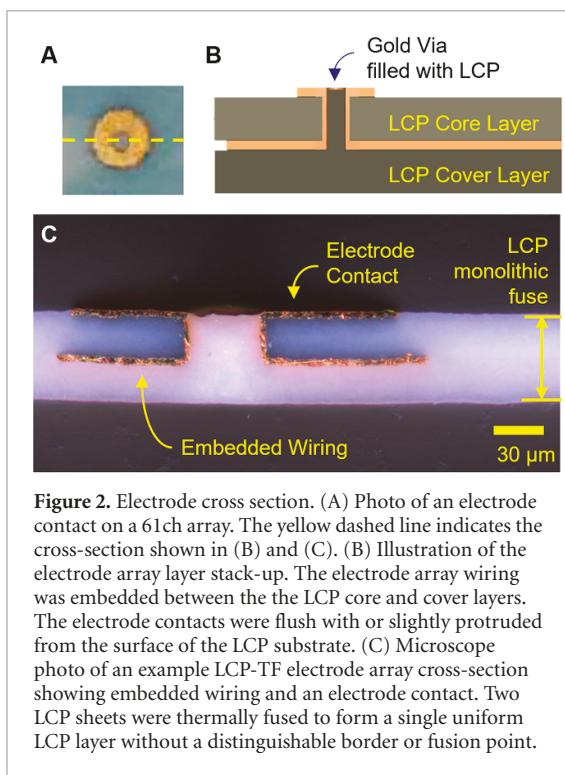


Figure 2. Electrode cross section. (A) Photo of an electrode contact on a 61ch array. The yellow dashed line indicates the cross-section shown in (B) and (C). (B) Illustration of the electrode array layer stack-up. The electrode array wiring was embedded between the the LCP core and cover layers. The electrode contacts were flush with or slightly protruded from the surface of the LCP substrate. (C) Microscope photo of an example LCP-TF electrode array cross-section showing embedded wiring and an electrode contact. Two LCP sheets were thermally fused to form a single uniform LCP layer without a distinguishable border or fusion point.

In addition, LCP has a higher working temperature than typical printed circuit board (PCB) material (FR-4) style laminates, good high frequency properties, high chemical resistance, and strong barrier properties [35]. This higher working temperature, combined with monolithic fusing of the LCP layers, allows our hybrid chronic implant design (80ch) to be sterilized using autoclaving. All of the LCP-TF electrodes can also be sterilized by ethylene oxide (EtO) or vaporized hydrogen peroxide sterilization (VHP).

2.1.2. Array design

The LCP-TF electrodes were fabricated with a minimal 2-metal layer design, where the electrode contacts were almost flush or slightly protruded from the LCP substrate to ensure good contact to brain tissue (figures 2(A) and (B)), rather than opening the top layer and having the electrode contacts recessed down in a well. Dyconex used conventional flexible PCB technologies and related equipment to fabricate these arrays. The fabrication steps started with the dual sided copper clad LCP sheet (Ultralam HT 3850, Rogers Corp.). The copper on the LCP sheet was etched off before applying the photoresist. Photolithography was performed to pattern the electrodes on the top layer and the wires on the bottom layer. Vias were laser-drilled to connect the electrodes to the wires on the bottom side. A thin palladium (Pd) seed layer was deposited and the resist structure was lifted from the substrate. Gold was electroplated on top of the Pd structures to the desired thickness. All processes were done on both sides of the LCP substrates simultaneously.

For improved flexibility, we used two of the thinnest LCP sheets commercially available (25 μm each). With heat (>280 °C) and pressure (>300 psi), a blank LCP sheet (Ultralam 3908, Rogers Corp.) was laminated to the bottom side of the substrate to encapsulate all of the wiring. Through this lamination process, the two LCP sheets were monolithically fused into a single layer, with gold (Au) wiring encapsulated in between (figure 2(C)). The interfaces between the LCP layers were not visible after fusing, preventing water ingress into the device from the edges, which is a common cause of delamination in polyimide devices, and a leading cause of device failure [36]. After fabrication, the total LCP-TF electrode thickness was just over 50 μm.

Only metals that are considered biocompatible (Au, PtIr and trace Pd) [37, 38] were used in the LCP-TF devices. *In vitro* tests showed LCP-TF electrodes meet biocompatibility criteria guided by ISO 10993-5 [39]. Implanting similar LCP-TF electrodes in rabbit retina for 2.5 years showed no adverse effects [34]. LCP-TF electrodes produced by Dyconex have successfully passed ISO 10993-5 [40].

The LCP-TF electrodes include much thicker (5 μm) Au layers than traditional TF devices (~0.1 μm). This reduces the resistance of the wires and improves their durability to surgical handling. A different LCP device design with thinner Au wires (500 nm) was bend tested to a 1 mm bend radius (nearly folding) and achieved 6000–12 000 bend cycles before failure [38]. The wire widths and spacings used ranged from 30/30 μm to 60/40 μm, respectively. The finer design (30/30 μm) was used where high density was required and wider wires and spacing (60/40 μm) were used wherever possible to minimize trace resistance and increase fabrication yield. The wire resistance for a 60 μm wide wire was ~7 Ω cm⁻¹.

Our microelectrode impedance was much lower and more uniform than microwire arrays [27] due to larger surface area (200 μm vs 40 μm dia.) and precise lithographic patterning of the electrode contacts. All electrode contacts were fabricated with gold as the base metal. Some arrays were electroplated with PtIr (Platinum Group Coating LLC), to reduce the electrode impedance [41, 42]. This electrode-deposited PtIr coating has demonstrated lower impedance, decreased noise, and increased signal-to-noise ratio (SNR) in chronic implants [43]. Immunohistochemistry showed no significant differences in the immune response between PtIr coated and uncoated electrodes [43]. The PtIr coating was applied at room temperature, making it easy to integrate with standard FPC manufacturing processes, a crucial design consideration for large-scale manufacturing.

We designed the LCP-TF electrodes so that no additional soldering or assembly was required to connect the electrodes with recording headstages. This

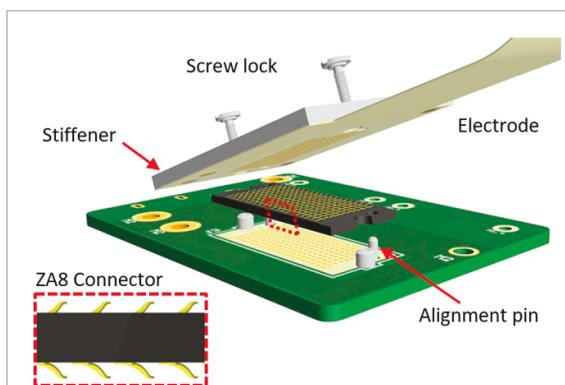


Figure 3. 3D illustration of the ultra-low profile, high-density (0.8 mm pitch) spring connector. The LCP-TF electrode array design included four alignment holes and a stiffener to increase the thickness and rigidity of the device in the connector area. The alignment holes and stiffener were standard features of the LCP flexible circuit process. (Inset) A side view of the spring connector highlighting the metal springs on the top and bottom of the connector.

substantially reduced the difficulty and cost of manufacturing. We used a FPC zero-insertion-force (ZIF, FH43B, Hirose Inc.) connector and an ultra-low profile, high-density (0.8 mm pitch) spring connector (ZA8, Samtec Inc.) (figure 3). The ZA8 is highly reliable and has demonstrated 100% connection yield and low resistance after 1000 connection cycles [44]. Both connectors only required a specified thickness of stiffening material added to the bottom of the connector region. Using standard high-density FPC connectors reduced the amount of post-processing required for the LCP-TF arrays.

2.2. Molding

For LCP-TF electrodes used in human intraoperative research, we have molded the electrode in medical grade silicone (MDX4-4210, Dow Corning) to provide soft, rounded edges [33, 45, 46], reducing the possibility of the thin LCP edges damaging the cortex during surgical placement. The molded device was $\sim 200 \mu\text{m}$ thick, $<30\%$ of the thickness of CG electrodes (AdTech, 850 μm). The silicone molding was also used to combine multiple LCP-TF electrodes, creating a single array with larger coverage and uniform contact spacing (supplement figure 1 (available online at stacks.iop.org/JNE/18/045009/mmedia)). We have used similar molding methods for NHP implants in prior studies [33, 47]. Additionally, the silicone molding can provide mechanical features, such as bending the cable arm to 90° to facilitate electrode placement during intraoperative recordings.

2.2.1. Array molding

The general array molding steps are shown in figure 4(A). We used water-soluble tape (5414, 3 M) to temporarily protect the electrode contacts during molding. A medical-grade silicone primer (MED1-161, Nusil) was used to strengthen the bond between

the LCP-TF and the silicone. A stainless-steel stencil, pre-treated with medical-grade demolding agent (MCC-DGF14 A, MicroCare Corp.) was used to control the shape and thickness of the silicone molding. Samples were heated to 60 °C to reduce the silicone curing time to 2 h. Finally, molded arrays were released by rinsing with warm (>40 °C) deionized (DI) water. This molding method achieved a nearly flush boundary between silicone and LCP at the device edges (figure 4(B)), yielding a flexible array that had a much flatter surface topography compared to CG electrodes (figure 4(C)). The electrode contacts were also nearly flush with the surface (figure 4(C)). In contrast, CG electrode contacts are recessed from the surface of the array by $\sim 200 \mu\text{m}$, potentially causing irritation to the brain from the unevenness of the surface features.

2.2.2. Forming the coiled leads

For the chronic array, the flat LCP-TF ribbon cabling, which carries micro-wiring from contacts to connector, must be converted to a round, flexible lead for proper tunneling and suturing during semi-chronic implantation. We achieved this by winding the LCP-TF ribbons around a 1.6 mm diameter steel core to form a coiled shape and then inserting the coil into a 2.8 mm outer diameter polyurethane tube (Nordson Medical). The metal winding core was removed, and the tube was filled with silicone to ensure that no empty space was left inside while keeping the lead round and flexible.

2.3. Array flexibility evaluation

To assess the maximum bending force that could be exerted on the brain by the electrodes, we conducted four-point flexural bending tests on LCP-TF and CG arrays. To account for any anisotropy, this bending test was done at three angles (0°, 45°, and 90°) on the horizontal plane of each array. These tests were repeated 12 times per array. With force and displacement data, we calculated the effective flexural modulus. This modulus was then used to determine the maximum force that an electrode array could exert on the brain. This was calculated assuming the array would have to bend to a radius of 60 mm, which was the smallest radius of curvature of an MRI brain scan obtained from the NIH 3D Print Exchange (Model 3DPX-000320). The mean maximum force values of each array were averaged across all angles and the standard deviation between the means of each angle were obtained. These results were then used to calculate the standard error of means for each sample. This was done to demonstrate both the average maximum force for each array and the range of maximum force each array could exert. We used this method to compare an FDA-approved commercially available ECoG electrode array (Ad-Tech Medical Instrument Corporation, FG64C-SP10X-000) and an LCP-TF device prototype without Au traces. More

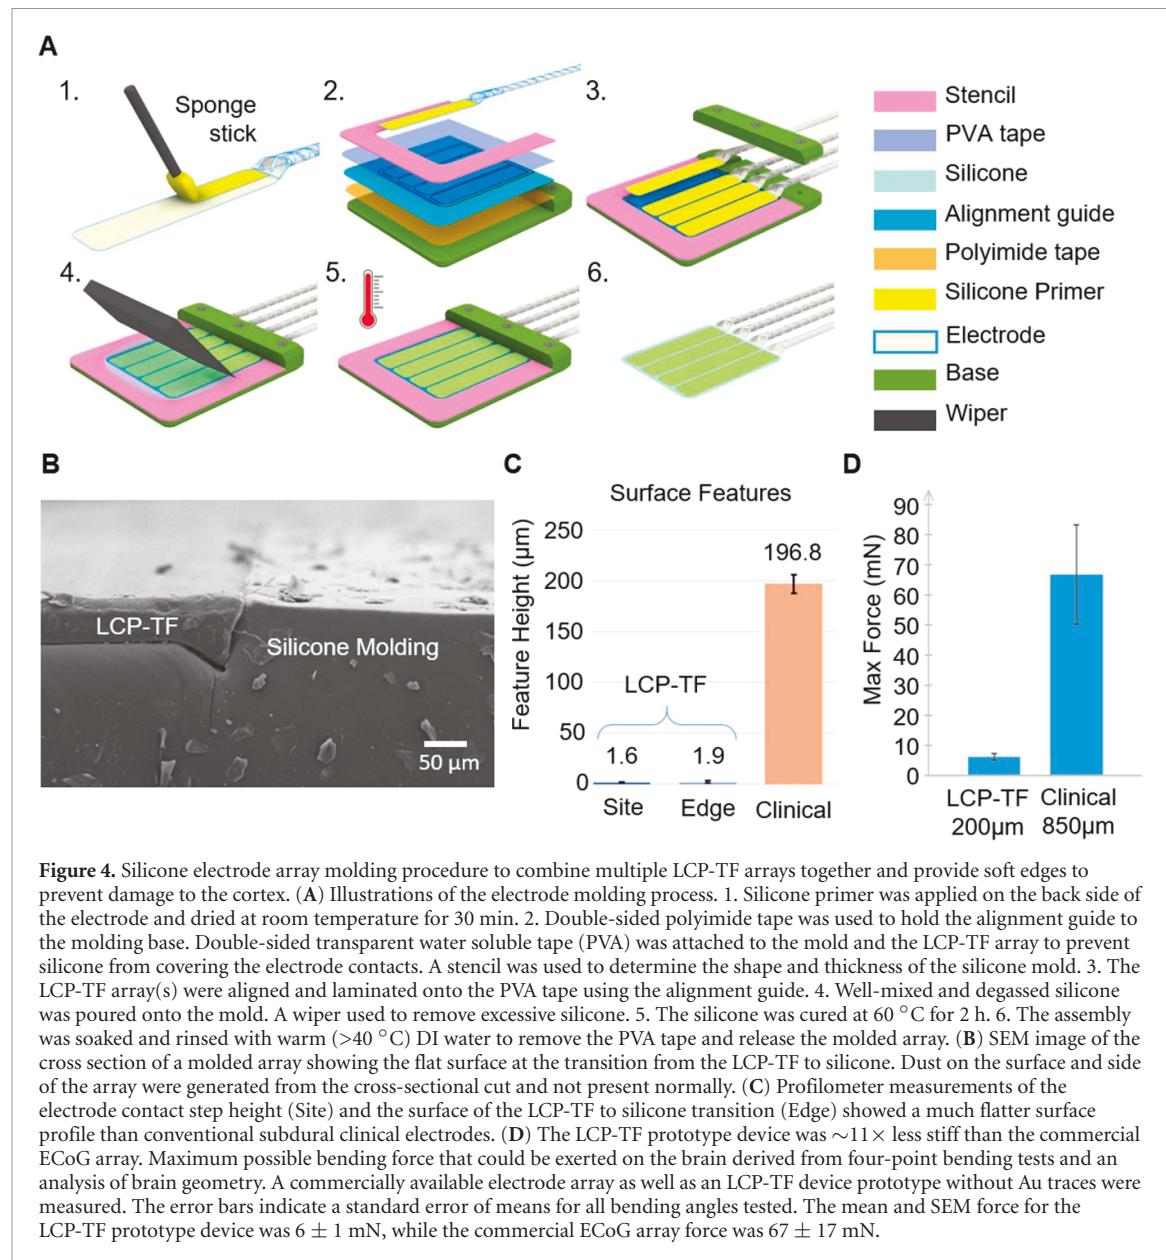


Figure 4. Silicone electrode array molding procedure to combine multiple LCP-TF arrays together and provide soft edges to prevent damage to the cortex. (A) Illustrations of the electrode molding process. 1. Silicone primer was applied on the back side of the electrode and dried at room temperature for 30 min. 2. Double-sided polyimide tape was used to hold the alignment guide to the molding base. Double-sided transparent water soluble tape (PVA) was attached to the mold and the LCP-TF array to prevent silicone from covering the electrode contacts. A stencil was used to determine the shape and thickness of the silicone mold. 3. The LCP-TF array(s) were aligned and laminated onto the PVA tape using the alignment guide. 4. Well-mixed and degassed silicone was poured onto the mold. A wiper used to remove excessive silicone. 5. The silicone was cured at 60 °C for 2 h. 6. The assembly was soaked and rinsed with warm (>40 °C) DI water to remove the PVA tape and release the molded array. (B) SEM image of the cross section of a molded array showing the flat surface at the transition from the LCP-TF to silicone. Dust on the surface and side of the array were generated from the cross-sectional cut and not present normally. (C) Profilometer measurements of the electrode contact step height (Site) and the surface of the LCP-TF to silicone transition (Edge) showed a much flatter surface profile than conventional subdural clinical electrodes. (D) The LCP-TF prototype device was ~11× less stiff than the commercial ECoG array. Maximum possible bending force that could be exerted on the brain derived from four-point bending tests and an analysis of brain geometry. A commercially available electrode array as well as an LCP-TF device prototype without Au traces were measured. The error bars indicate a standard error of means for all bending angles tested. The mean and SEM force for the LCP-TF prototype device was 6 ± 1 mN, while the commercial ECoG array force was 67 ± 17 mN.

details about the testing setup and procedure as well as a more detailed analysis of these and other relevant material samples can be found in another study [48].

We compared the stiffness of the molded chronic array mechanical prototype (200 μm thick total, no Au wires) to an FDA-approved, conventional ECoG electrode array (Ad-Tech) through a four-point flexural bending test setup. The LCP-TF prototype device was ~11× less stiff than the commercial ECoG array. The mean and SEM force for the LCP-TF prototype device was 6 ± 1 mN, while the commercial ECoG array force was 67 ± 17 mN (figure 4(D)).

2.4. Data acquisition system

Long wires between microelectrodes and the recording system can cause signal distortions and increased noise [27]. Commercially available headstages amplify and digitize 32–64 channels simultaneously but

are not designed to scale up to record hundreds or thousands of channels. Therefore, we have designed a modular adapter system with a miniature digitizing headstage using a 64-channel digital electrophysiology integrated circuit (RHD 2164, Intan Technologies LLC). Our 64-channel digitizing headstage was compact, 19 × 20 mm, and weighed 2.0 grams (figure 5(A)). The small size and light weight of the digitizing headstage made it suitable for use in freely behaving rat experiments as well as larger animals and humans. The digitizing headstage was connected to different modular adapter boards, which were designed to minimize the physical footprint and enable daisy chaining multiple headstages together to reduce the number of connections required during intraoperative experiments (figure 5(B)). We used standard micro-HDMI cables to enhance reliability and accessibility. For the back-end acquisition system, we modified the Intan 1024ch controller (C3008,

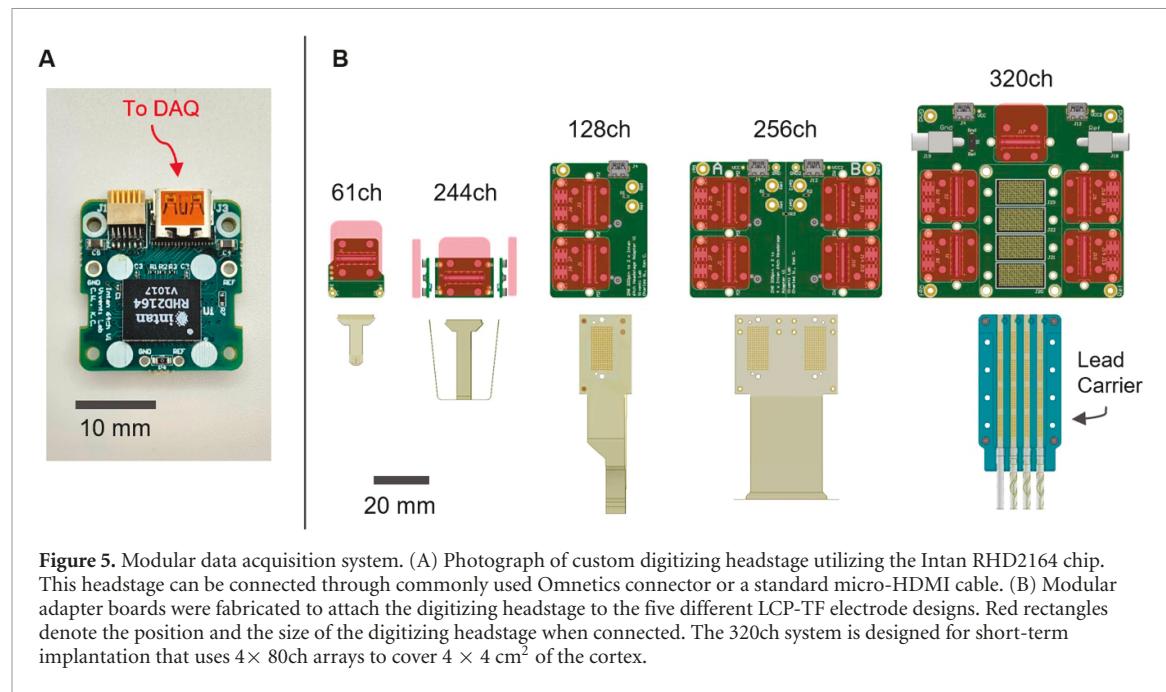


Figure 5. Modular data acquisition system. (A) Photograph of custom digitizing headstage utilizing the Intan RHD2164 chip. This headstage can be connected through commonly used Omnetics connector or a standard micro-HDMI cable. (B) Modular adapter boards were fabricated to attach the digitizing headstage to the five different LCP-TF electrode designs. Red rectangles denote the position and the size of the digitizing headstage when connected. The 320ch system is designed for short-term implantation that uses 4×80 ch arrays to cover $4 \times 4 \text{ cm}^2$ of the cortex.

Intan Technology) to be powered with an external DC battery to reduce power line noise (60 Hz) and to eliminate any connection to AC power for additional electrical safety (supplement figure 2). The 1024ch controller additionally includes galvanic isolation of the power and data lines for each headstage port. The complete DAQ system was approved by the Duke University Hospital Clinical Engineering and NYU Langone Hospital Clinical Engineering departments.

2.5. Stimulation experiment

Three 61ch LCP-TF arrays with PtIr electrode coatings were evaluated for electrical stimulation. The arrays were tested *in vitro* in 0.9% saline. We used a multichannel recording and stimulation system to deliver stimulation and measure electrode impedance (RHS 128-channel stimulation/recording controller system and RHS 32-channel headstage, Intan Technology). One million biphasic current pulses (124 μA , 200 μs per phase, cathode first, 40 Hz repetition rate) were applied to four selected channels on each 61ch array. A total of 12 channels were tested. The initial and final impedance measurements were taken at nine different frequencies of 75, 100, 200, 400, 500, 800, 1000, 2000, and 4000 Hz.

2.6. Intraoperative experiments

We have recorded from multiple participants using our high-density, molded, LCP-TF electrode arrays placed subdurally over the surface of the brain for up to 30 min during epilepsy surgery, brain tumor resection, or deep brain stimulator (DBS) placement. Participants gave their written informed consent before the day of the surgery. All participants were fluent in English. All protocols were approved by the Duke Health and NYU Langone Institutional Review

Board. All experiments and data in this study complied with all relevant ethical regulations. Electrodes with holders were sterilized with EtO at Duke Hospital or VHP at NYU Langone Hospital.

In this paper, we report the data from two participants. One participant, a 20 year-old female, heard a series of words and non-words during an asleep craniotomy for seizure focus resection. μ ECoG signals were recorded using a 244ch array placed over the posterior superior temporal gyrus (pSTG), while the participant passively listened to 336 words and non-words (randomized into four blocks of 84 trials). Data were acquired at a sampling rate of 20 000 samples per second (SPS).

The other participant, a 42 year-old male, performed a directed finger movement task during an awake craniotomy for brain tumor resection. The participant wore a 5DT Data Glove (Fifth Dimension Technologies, Orlando FL), used to record finger kinematics, on the contralateral hand, while performing the task. The μ ECoG signals were recorded by a 244ch array over the 'hand-knob' region of the motor cortex. A presentation laptop was used to cue the patient to flex the appropriate finger repeatedly until a rest period followed by a new cue (finger). The overall experiment contained 75 trials (randomized into three blocks) with 15 trials per finger. Each trial contained up to 5 s of finger movement.

2.6.1. Recording system for open craniotomy experiments

For intraoperative recordings in epilepsy or brain tumor surgery, we utilized a modified METRx™ flexible arm (Medtronic, St. Paul, MN) to hold the 244ch LCP-TF electrode deployment system (figure 6(A)). The system was slowly lowered down

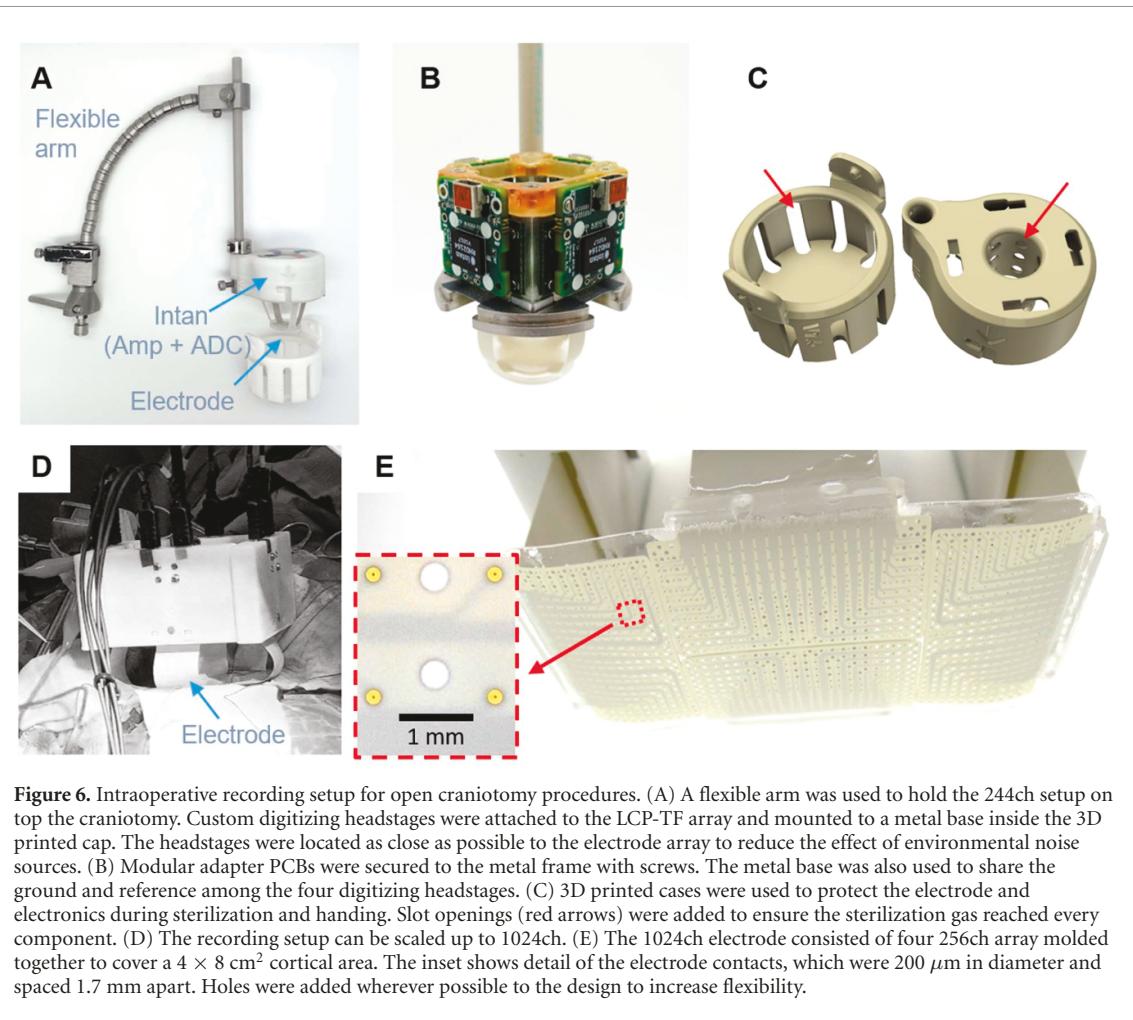


Figure 6. Intraoperative recording setup for open craniotomy procedures. (A) A flexible arm was used to hold the 244ch setup on top of the craniotomy. Custom digitizing headstages were attached to the LCP-TF array and mounted to a metal base inside the 3D printed cap. The headstages were located as close as possible to the electrode array to reduce the effect of environmental noise sources. (B) Modular adapter PCBs were secured to the metal frame with screws. The metal base was also used to share the ground and reference among the four digitizing headstages. (C) 3D printed cases were used to protect the electrode and electronics during sterilization and handling. Slot openings (red arrows) were added to ensure the sterilization gas reached every component. (D) The recording setup can be scaled up to 1024ch. (E) The 1024ch electrode consisted of four 256ch array molded together to cover a $4 \times 8 \text{ cm}^2$ cortical area. The inset shows detail of the electrode contacts, which were 200 μm in diameter and spaced 1.7 mm apart. Holes were added wherever possible to the design to increase flexibility.

for the electrode to make contact with the cortical surface (supplemental movie 1). Spring tension in the arm prevented excessive force from being transmitted to the brain. The deployment system structure was made out of stainless steel, machined in house. The stainless steel base provided an electrical connection to bridge the reference and ground connections for each of the four digitizing headstages together (figure 6(B)). A 3D printed housing, made out of biocompatible material (Duraform PA, 3D System), protected the electronics and enabled easy handling of the system during surgery. Slot openings were included in the housing to allow sterilization gas to reach the internal components (figure 6(C)). The same design principles were used to scale to 1024 channels (figures 6(D) and (E)). We have successfully used this open-craniotomy intraoperative recording setup 21 times.


2.6.2. Recording system for DBS experiments

To record from the cortex in patients undergoing DBS surgery, we made a flexible, long, and narrow LCP-TF electrode (128ch). The LCP-TF electrode was inserted through a small, 14 mm diameter burr-hole and advanced more than 80 mm away from the burr-hole site along the cortical surface (figures 7(A) and

(B)). We designed a mechanical holding structure that was integrated with NexFrame stereotactic system (Medtronic, St. Paul, MN) (figure 7(C)). The system is also adaptable to other methods of DBS implantation (e.g. frame based stereotaxy). The tip of the LCP-TF electrode was also molded with an extra silicone pocket to temporarily hold a malleable brain retractor device (R8960, T. Fukushima Brain Spatulas, Integra) to facilitate subdural array tunneling and navigation (figure 7(D)). The 128ch LCP-TF electrode included a ruler on the back side of the array to assist in targeting when sliding under the dura (figure 7(E)). The ruler was printed with a biocompatible solder mask (NPR-80, Nippon Polytech Corp.). Electrode placement was verified during intraoperative computerized tomography acquisition which was used to confirm DBS lead placement. Up to the day of submission, we have deployed this array design four times intraoperatively during DBS surgeries.

2.7. Data analysis

In both auditory and motor experiments, the recordings from each channel were subjected to common-average-referencing to remove line noise. We rejected electrode channels from the common average with

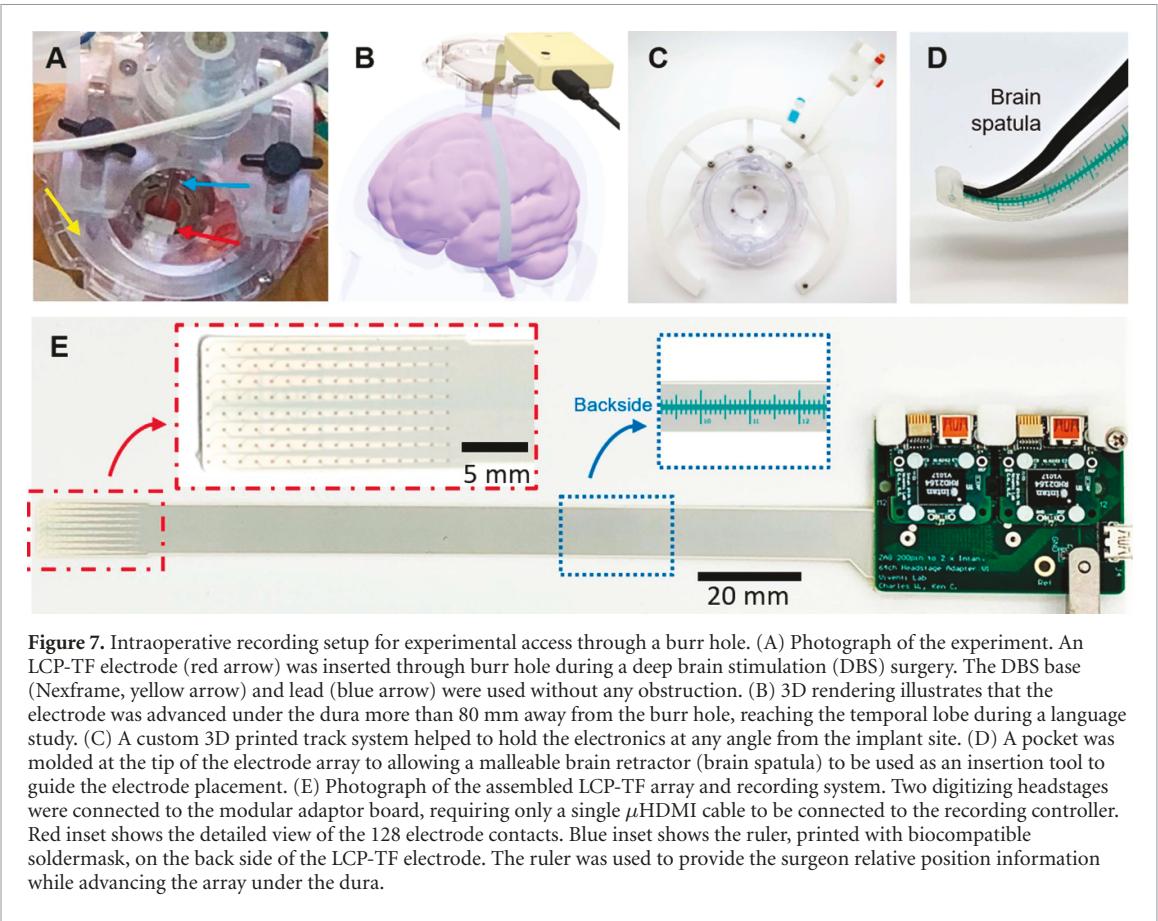

high impedance ($>1 \text{ M}\Omega$). To display data spatially, we predicted noiseless neural potential fields using Gaussian process modeling of the electrode recordings [49]. To adapt to time-varying spatial statistics, spatial covariance kernels were updated at latent state transitions, which were estimated by hidden Markov modeling of the average signal power envelope.

2.7.1. Spectrogram analysis

To examine spectral features in each electrode, we computed spectrograms for each channel. We decomposed the data into time-frequency components using a multi-taper spectral analysis with a 500 ms analysis window (50 ms time steps) and 10 Hz frequency smoothing [50]. We then normalized the spectrograms by computing the average $1/f$ spectral estimate during the baseline period ($-0.5\text{--}0$ s before auditory onset) across all trials and dividing the spectral time steps by the mean estimate for each frequency band.

2.7.2. High gamma extraction and electrode significance

We used the high-gamma (HG: 70–150 Hz) band to characterize the neural response from our LCP-TF electrode, as it has shown to be a local index of cognition and a strong correlate of multi-unit firing [51–53]. From previously established methods, we used IIR filters to filter data into eight frequency bands between 70 and 150 Hz [54]. We computed

the envelope of each band using the Hilbert transform and then averaged the resultant envelopes across all bands to create a total envelope. Finally, we down sampled the filtered HG band to 200 Hz and normalized (z-scored) the envelope from the baseline responses ($-0.5\text{--}0$ s post stimulus onset) across all trials.

To assess electrode significance, we computed the average HG power (unnormalized) across trials in two time regions ('baseline' and 'response') of interests for each trial. For the auditory experiment, we defined 'baseline' as the 500 ms time window prior to auditory onset and 'response' as the time window from 250 to 750 ms post onset. For the finger flexion tasks, 'baseline' was defined as the 500 ms window prior to stimulus onset during which no finger movement was observed, and 'response' was defined as $-250\text{--}250$ ms centered around flexion onset. We identified statistically significant channels by comparing the power between baseline and response using a 10000 iteration one-sided empirical permutation test [55]. We corrected the significance across electrodes to an alpha level of 0.05 with the false discovery rate procedure [56] (one-sided FDR corrected, $P < 0.05$).

2.7.3. Linear decoder for finger flexion analysis

We used a previously established linear classification scheme to decode finger stimulus conditions from HG responses [57, 58]. Normalized HG

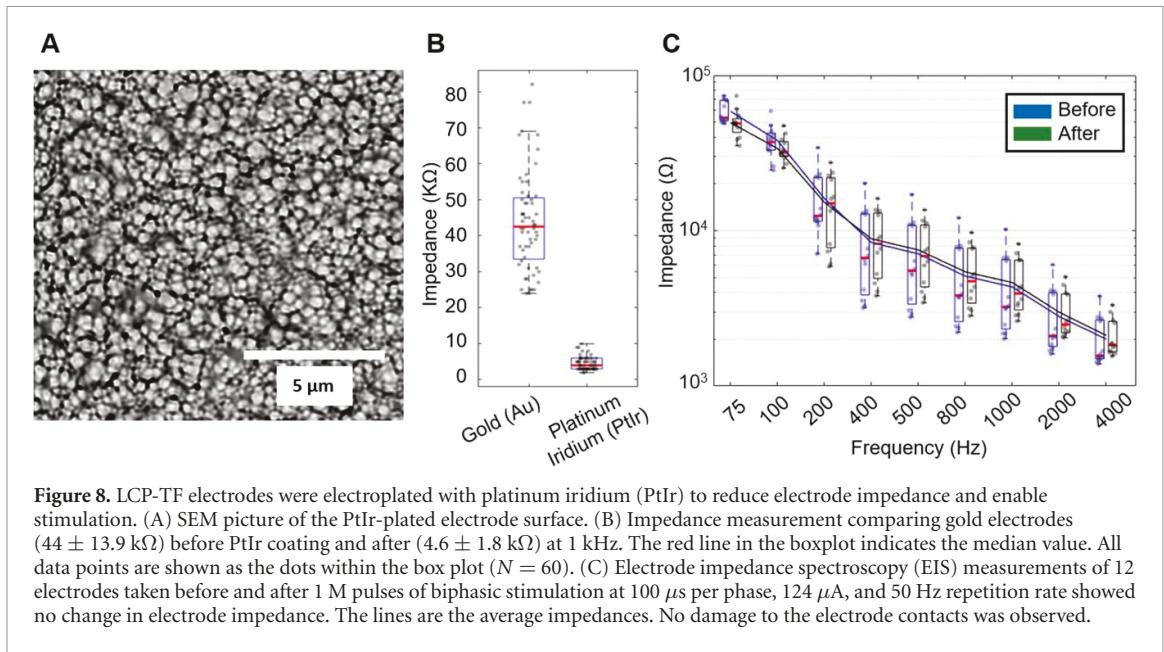


Figure 8. LCP-TF electrodes were electroplated with platinum iridium (PtIr) to reduce electrode impedance and enable stimulation. (A) SEM picture of the PtIr-plated electrode surface. (B) Impedance measurement comparing gold electrodes ($44 \pm 13.9 \text{ k}\Omega$) before PtIr coating and after ($4.6 \pm 1.8 \text{ k}\Omega$) at 1 kHz. The red line in the boxplot indicates the median value. All data points are shown as the dots within the box plot ($N = 60$). (C) Electrode impedance spectroscopy (EIS) measurements of 12 electrodes taken before and after 1 M pulses of biphasic stimulation at $100 \mu\text{s}$ per phase, $124 \mu\text{A}$, and 50 Hz repetition rate showed no change in electrode impedance. The lines are the average impedances. No damage to the electrode contacts was observed.

time-segments (length T) during response conditions were concatenated from significant channels (S sites) as feature vectors (length—ST) for each finger trial. The ST feature vectors were *z*-score normalized and compressed using singular value decomposition (SVD) with leave-one-out cross-validation. Finally, the singular scores from the compressed training-set were used to build a supervised linear discriminant (LD) model to decode finger conditions. To validate the model, the ST features of the test-set were compressed using the trained-SVD model and the corresponding scores were used to predict finger flexions using the supervised LD model. The optimal number of SVD components were obtained using nested cross-validation for each training-test set and the overall accuracy was estimated from the percentage of total correct predictions. We trained two different models: one to decode five-fingers (five-way) and another for three-finger (three-way, thumb, index, and little) movements.

3. Results

3.1. Stimulation capability

The electrode contacts were electroplated with PtIr. PtIr coatings are highly fractal and exhibit pseudo-capacitive reactions, dramatically increasing the electrode surface area [41, 42] (figure 8(A)), and thus decreasing contact impedance by an order of magnitude, from $44 \pm 13.9 \text{ k}\Omega$ to $4.6 \pm 1.8 \text{ k}\Omega$ at 1 kHz (figure 8(B)). This lower impedance provided an improved SNR [43] and enabled stimulation. A total of 12 channels in three arrays were tested with one million biphasic current pulses ($124 \mu\text{A}$, $200 \mu\text{s}$ per phase, cathode first, 40 Hz repetition rate). PtIr coated electrodes showed no degradation after one million pulses at twice the clinical neural stimulation

safety limit ($30 \mu\text{C cm}^{-2}$) [59] (figure 8(C)). We further tested the maximum current limit placed through the electrodes without causing damage. The maximum current we arrived at without overshooting the compliance limit setting was 1.275 mA ($200 \mu\text{s}$ per phase, cathode first, 40 Hz repetition rate). The microelectrodes showed no sign of degradation after one million pulses at 1.275 mA as well. The impedances, at 1 kHz, of the contacts before and after one million pulses at 1.275 mA were $6.6 \pm 1.3 \text{ k}\Omega$ and $5.8 \pm 0.7 \text{ k}\Omega$ ($N = 6$), respectively. Although the clinical safety limit for microelectrode stimulation is still undecided, this higher stimulation current is still below the Shannon limit ($k = 1.85$) [59] and has been used in animal research [60, 61].

3.2. High resolution recording

We report the data from two participants demonstrating the utility of high-resolution recording. In the first case, we used our 244ch LCP-TF array to record neural responses from the pSTG of an anesthetized patient by presenting an auditory stimulus (figure 9(A)). Uniform *in vivo* impedance measurement was observed in this experiment (supplement figure 3). We removed noisy single trials for each channel by identifying trials with absolute voltage amplitudes that exceed ten times the standard deviation. Spectral analysis of the recordings demonstrated an increase in the power of high gamma band (75–150 Hz) neural signals during auditory onset (figure 9(B)). The plotted area contains 244 channels, covering a total area of $12 \times 12 \text{ mm}^2$, and each electrode demonstrates a different neural response profile in the HG band. We examined the significance of our μ ECoG channels by comparing the HG power from auditory onset with respect to baseline. The one-sided permutation test identified 108 channels


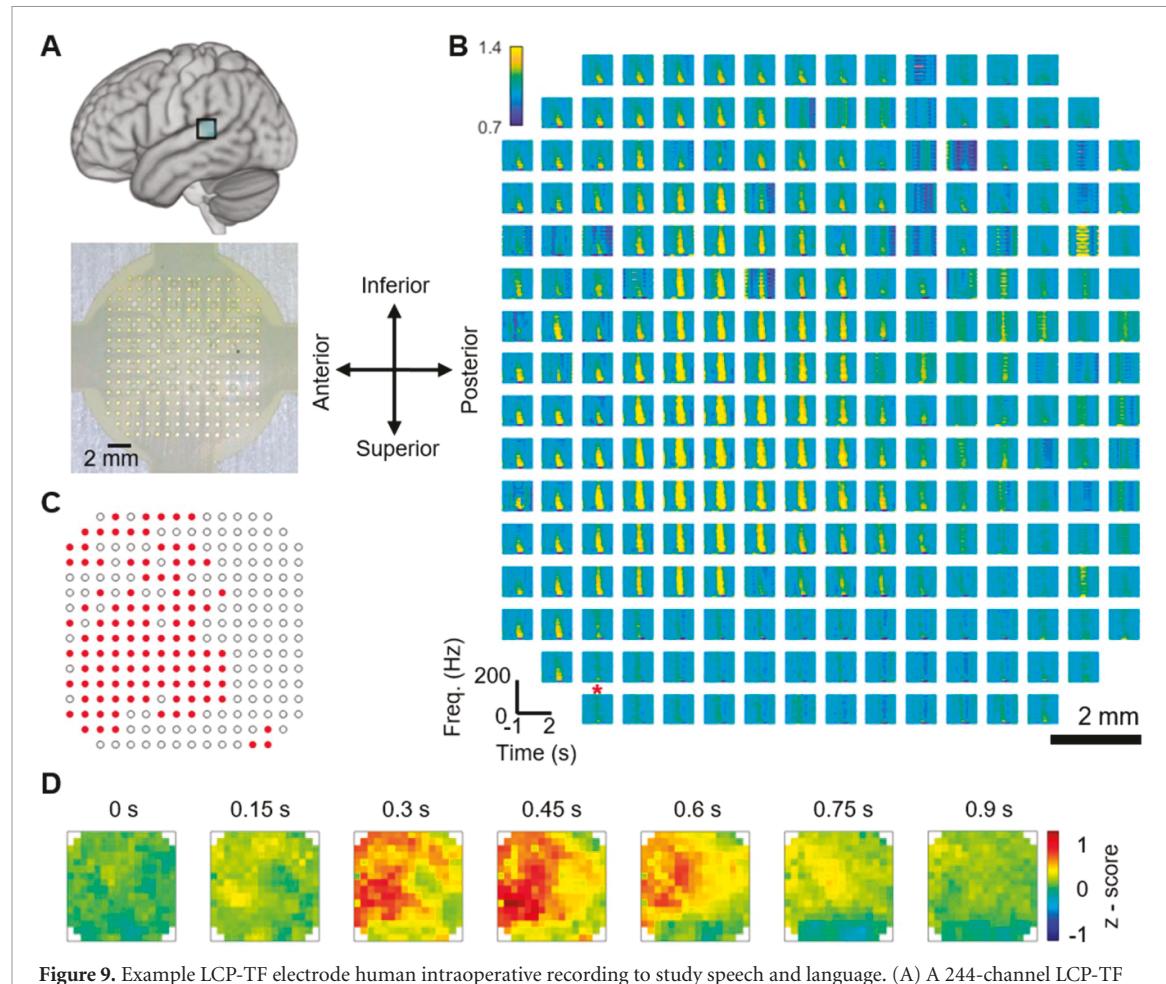


Figure 9. Example LCP-TF electrode human intraoperative recording to study speech and language. (A) A 244-channel LCP-TF electrode array (bottom) recorded auditory responses from the posterior superior temporal gyrus (pSTG—top) in a patient undergoing treatment for pharmacologically resistant epilepsy. The patient was asleep during the auditory stimulus (words and non-words) presentation. The *in vivo* electrode impedance data can be found in supplemental figure 3. (B) Spectrograms for the local field from each channel (right) show auditory responses on selective channels. These responses were mainly found in the high gamma (HG) frequency range (70–150 Hz), shown to be a correlate of multi-unit neuronal firing. The red star denoted the high impedance channel. (C) The red channels exhibit significant high-gamma responses during auditory onset relative to baseline (one-sided permutation test, $p < 0.05$, FDR corrected). (D) Normalized HG time-series heat maps show the spatial detail of the auditory response.

(out of 244, $p < 0.05$) with significant HG power and revealed a spatial pattern within the 16×16 grid (figure 9(C)). Further, our 244ch array showed a clear spatiotemporal progression of auditory processing at high resolution in pSTG (figure 9(D)). This spatio-temporal activation pattern occurred over a total of area of less than $12 \times 12 \text{ mm}^2$, indicating a pattern that would only be detectable by μ ECG as contacts on standard CG arrays are too large (2.3 mm diameter) and spaced too far apart (10 mm) to detect neural activation patterns at this spatial scale.

In the second case, we recorded motor neural responses using a similar 244ch LCP-TF array from the ‘hand-knob’ area in the motor cortex during a finger movement task (figure 10(A)). The finger kinematics were recorded using a data glove (figure 10(B)). Although this array contained some higher impedance channels (supplement figure 4), we found clear motor responses in the high-gamma band that had a spatial organization (figure 10(C)). Our statistical analysis identified 24 channels with

significant HG power, mostly grouped at the top-right corner of the array (figure 10(D)) and were used in the decoding analysis. Normalized HG responses revealed finger related activity indicating a clear, distinctive spatial-temporal organization of motor processing, with respect to the five fingers, within the 8×8 grid (figure 10(E)). The top right corner also appeared to react most strongly when the thumb was instructed to move. To demonstrate the decoding potential of our array, we used the HG responses from the above 24 sites to classify finger movements using a linear discriminant classifier, as described in section 2. In the five-finger decoding, the classifier was successful in identifying the finger types with an average decoding accuracy of 61% (chance 20%), with maximum decoding accuracies for the thumb. Further analysis indicated that the increased classification error between middle, ring, and little finger, were caused by natural co-contraction [62], where multiple fingers move together when only a single finger was instructed to move. These natural

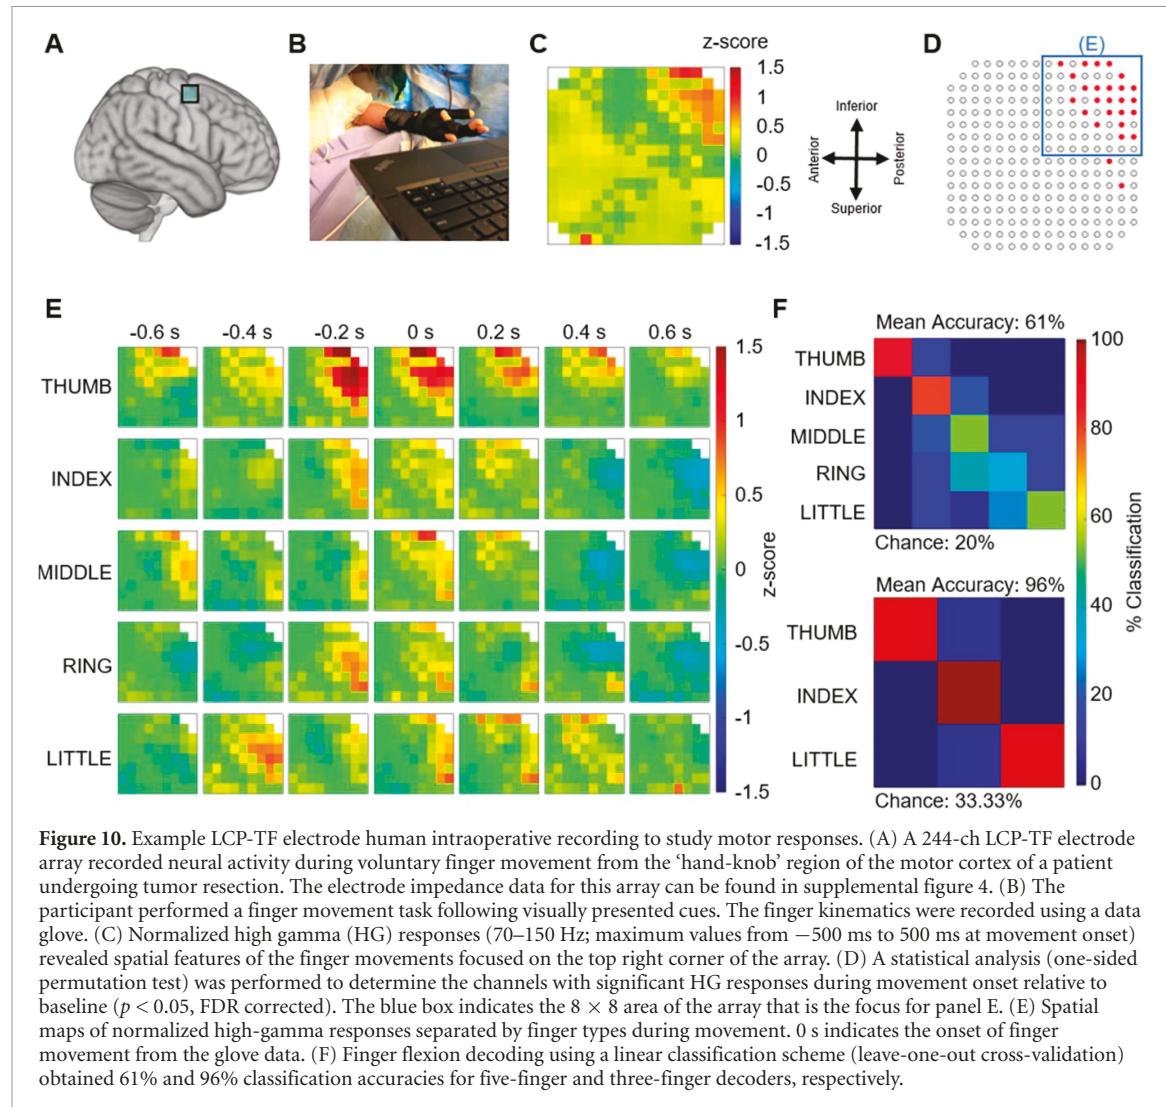

co-contractions were confirmed by increased glove kinematic correlations between the middle, ring, and little finger (supplementary figure 5). To examine flexion analysis between independent finger articulations, we then reduced the analysis to a three-way decoder to classify between thumb, index, and little finger, which yielded an average decoding accuracy of 96% (chance 33.33%) (figure 10(F)). This nearly perfect decoding was achieved in a predominantly thumb responsive area of cortex. These 244ch array intraoperative recordings demonstrate the ability of our LCP-TF arrays to record and decode auditory and motor information at high resolution.

3.3. Chronic array

We have designed high-resolution electrodes for epilepsy pre-surgical evaluation. This LCP-TF design is intended for semi-chronic implants up to 30 d. For clinical use, it is important to maintain the clinical standard macro-electrodes, in addition to the micro-electrodes. Further, the electrode cables must be passed through a standard cannula (3 mm dia.). Round cables are preferred to allow surgeons to suture

and seal the dura and scalp around the cables (see section 2.2.2).

Here we show an LCP-TF design which meets these criteria (figures 11(A) and (B)). We have designed an 80ch hybrid LCP-TF array with 76 research micro-electrodes interspersed amongst four macro-electrodes of clinical-standard size and spacing. While other TF electrodes use flat ribbon cables that cannot be implanted by standard surgical procedures, our LCP-TF array has rounded leads that neurosurgeons consider acceptable for short-term (<30 d) implantation. The planar TF-LCP cables are molded into helically wound leads of 2.8 mm diameter without sharp edges to allow longitudinal elongation (up to 15%) (figure 11(C) and section 2.2.2). These leads are similar to existing CG electrode leads and can be tunneled through the skin as in current surgeries but contain 5–10× more channels than traditional CG electrode leads. In addition, when combining multiple arrays to a 4×4 cm coverage, we have developed a novel, high-density connector system where all percutaneous leads will be inserted into a custom lead carrier that provides easy placement and guaranteed alignment with the

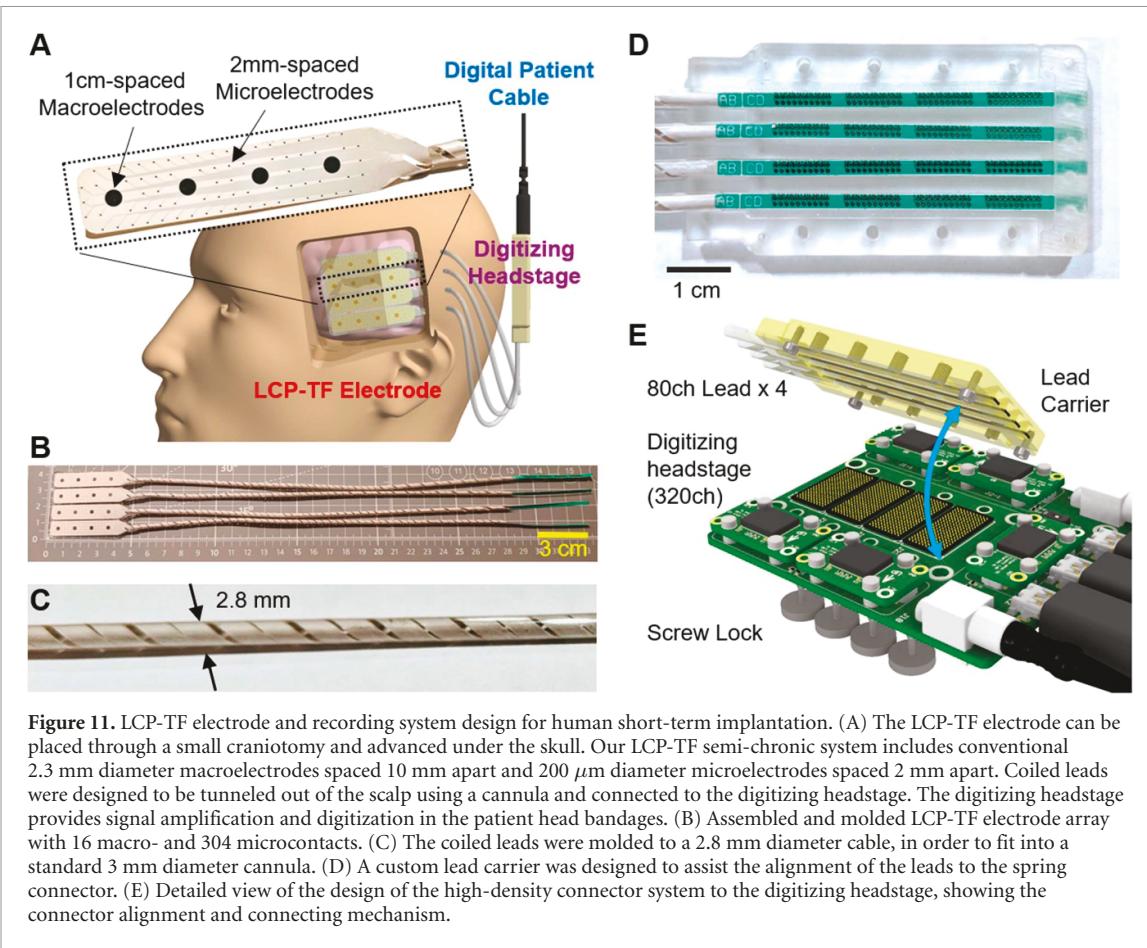


Figure 11. LCP-TF electrode and recording system design for human short-term implantation. (A) The LCP-TF electrode can be placed through a small craniotomy and advanced under the skull. Our LCP-TF semi-chronic system includes conventional 2.3 mm diameter macroelectrodes spaced 10 mm apart and 200 μ m diameter microelectrodes spaced 2 mm apart. Coiled leads were designed to be tunneled out of the scalp using a cannula and connected to the digitizing headstage. The digitizing headstage provides signal amplification and digitization in the patient head bandages. (B) Assembled and molded LCP-TF electrode array with 16 macro- and 304 microcontacts. (C) The coiled leads were molded to a 2.8 mm diameter cable, in order to fit into a standard 3 mm diameter cannula. (D) A custom lead carrier was designed to assist the alignment of the leads to the spring connector. (E) Detailed view of the design of the high-density connector system to the digitizing headstage, showing the connector alignment and connecting mechanism.

ZA8 spring connectors (described in section 2) (figures 11(D) and (E)).

4. Discussion

We have successfully demonstrated the ability to record from LCP-TF electrodes in rodents, NHPs, and humans. This has been accomplished through advances in design, fabrication, and implementation. In the current work, we demonstrate this ability in human recordings from two participants performing a passive listening task and a finger movement task. Micro-scale spatio-temporal neural activation patterns were shown in both the auditory (pSTG) and motor (hand motor cortex) brain regions.

While these results of our initial experiments in rodents, NHPs and humans are promising, much work remains to be done. This includes (a) developing LCP-TF electrodes to record from deep brain structures, (b) further increasing the spatial resolution of the electrodes, (c) performing required safety and biocompatibility studies for FDA 510(k) approval, and (d) exploring applications of LCP-TF electrodes to cognitive, motor, visual, and auditory prostheses.

Recently, stereo-electroencephalographic (SEEG) electrodes have been increasingly adopted for seizure monitoring. The resurgence of SEEG compared to

ECoG is largely attributable to the reduced inflammation, infection and pain using robotic minimally invasive surgical techniques [63]. Our LCP-TF technology could be applied to SEEG as well. As a proof of concept, we have developed a 61ch LCP-TF SEEG electrode that included both micro- and macroelectrodes, similar to other efforts [64]. Our LCP-TF SEEG electrode was rolled and molded into a cylindrical shape only \sim 900 μ m in diameter (figure 12), the same form factor as clinical-standard SEEG arrays. Our LCP-TF SEEG electrode could be used to record from deep brain structures as well as cortical structures, though more testing and validation of this design is required. Future work will focus on demonstrating the functionality, safety, and efficacy of the LCP-TF SEEG design.

We have recently determined that sub-millimeter electrode density is required to reliably sample neural activity in multiple species including human [49]. Using spatial analysis ('kriging' [65]), we established the effect of sampling density on interpolation error, and determined the kriging resolution required for $<10\%$ interpolation error in 95% of cases [49]. The required spacing varied across species, and across temporal bandpass. In a noise-free setting, the spacing needed to sample high frequency activity (75–300 Hz) in human auditory cortex under anesthesia was 622 μ m. While our initial LCP-TF electrodes have a range of 0.42–2 mm spacing, this result indicates

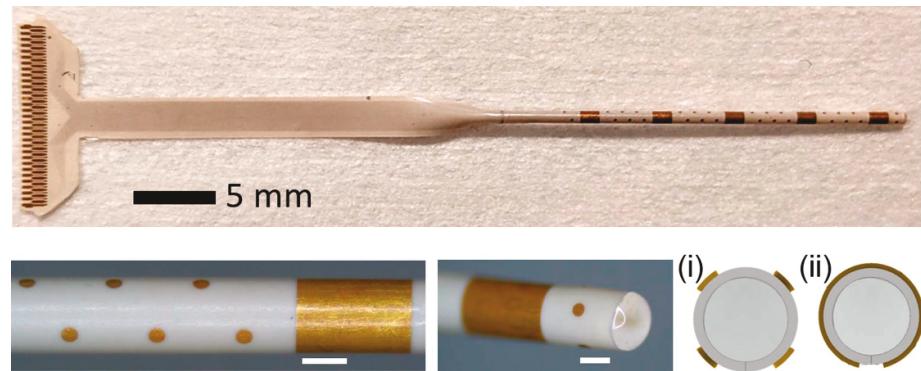


Figure 12. LCP-TF SEEG prototype includes 56 microelectrodes with $500\ \mu\text{m}$ spacing and five macroelectrodes with $5\ \text{mm}$ spacing. The physical form factor is the same as standard clinical SEEG electrodes ($900\ \mu\text{m}$ diameter), making it compatible with existing clinical workflows. Cross sectional drawings illustrate the arrangement of four microelectrodes around the circumference of the array (i), while the macroelectrodes wrap around the entire array (ii).

that further increases in sampling density will likely be required. However, the LCP-TF arrays described here provide an important step towards high-resolution neural interfaces before the next generation of electrodes with embedded flexible electronics [66–68] are fully tested and available for clinical use.

Our LCP-TF recordings and other microelectrode recordings over the past 10 years [10–13, 15–19] have revealed a striking heterogeneity in the spatiotemporal dynamics of interictal epileptic events including HFOs, interictal discharges, and microseizures. However, all of these studies have been limited by their inability to observe microscale dynamics of human epileptic cortex simultaneously at high resolution and with large cortical coverage. To further relate these high-resolution electrophysiological events to clinical events like seizure initiation, propagation, and termination, researchers need to be able to implant our LCP-TF electrodes over the putative seizure onset zone and then obtain continuous recordings in the epilepsy monitoring unit. Such a clinical study is not possible without FDA approval of the electrodes. Our LCP-TF electrode design contains conventional macroelectrodes for clinical care and microelectrodes for research. Our next step will be to perform the required biocompatibility and safety studies to obtain FDA 510(k) clearance for short-term ($<30\ \text{d}$) implantation.

A critical advantage of our LCP-TF electrodes over existing technologies is their low cost compared with standard clinical electrode arrays. The LCP-TF electrodes cost half as much per square centimeter compared to conventional clinical arrays and other alternatives. CGs typically come in 4–10 channel strip and 8–96 channel grid configurations. Typical sales prices for these devices range from \$450 to \$1400. We used technologies that are designed to compete with high volume printed circuit board manufacturing. Our LCP-TF effective cost was $\sim \$4\ \text{cm}^{-2}$ including the lead and connector, which is often not included in cost comparisons.

Increased availability of high-resolution electrodes will facilitate the broad collection of high-resolution neural data from humans for many applications, including better informing seizure diagnostics [7, 13, 15, 69–72], improved therapies for motor disorders and enhanced prosthetic systems. We have already started disseminating the LCP-TF electrodes described in this paper to more than ten labs and will continue to make our technology available for broader investigative use. Our platform technology can be adapted for patients with sensory and motor deficits treated with penetrating microelectrodes in proof-of-concept brain-machine interfaces as well. Exploratory studies in epilepsy patients with high rates of mood and memory symptoms [73] can extend this technology to study mood and cognitive disorders.

Higher resolution electrode arrays will also enable improved motor brain-machine interfaces [5, 23–26], visual [74], auditory prostheses [23, 75–81], and enhanced research of cognition [22]. High resolution recordings will be increasingly important for the next generation of therapeutic and prosthetic neural devices [82–86]. In each case, high-resolution recording and stimulation is required. Our system will achieve these goals by increasing spatial resolution, while maintaining clinically relevant coverage, using a thinner and more efficient electrode and cabling system.

5. Conclusion

In this paper, we have developed a platform technology to enable high-resolution cortical interfacing, in a form factor that is scalable, cost effective, and compatible with current clinical care. We demonstrated LCP-TF electrodes and supporting system designs suitable for animal and human research. The LCP-TF electrodes were designed to cover a wide range of research subjects, recording densities, and spatial coverages. Silicone molding allowed us to combine

multiple arrays to further extend the spatial coverage. The mechanical deployment hardware positioned the amplifier and digitizer very close to the electrodes, reducing the effect of environmental noise sources. We have already shared many of these devices for animal use and are preparing for broader dissemination to many more interested users. Dissemination of our high-resolution LCP-TF electrodes will lead to a significant acceleration of research progress and offer powerful insights into human brain activity.

Data availability statement

The data generated and/or analysed during the current study are not publicly available for legal/ethical reasons but are available from the corresponding author on reasonable request.

Acknowledgments

The cartoon icons in Figure 1 are from www.biorender.com.

Grant #DoD EP200077, NIH U01 NS099697, NSF CBET-1752274, NIH CTSA grant UL1TR002553 and Find A Cure for Epilepsy and Seizures (FACES).

Author contribution: CHC, CW, KB, and JV designed and tested the electrode setup and custom hardware. MW, VW, and BB performed initial development and pilot experiments. CHC and IR fabricated SEEG prototype devices in the cleanroom. EB provided the LCP electrode cross-section photo and early material biocompatibility data. NSW, TO, CFR, and FS performed array flexibility evaluation. AD, KEW, and BP performed stimulation testing. CHC, MT, SD, KB, GC, and JV analyzed and interpreted the data. CHC, KB, SR, SD, BP, GC, and JV collected data. SR, WD, DF, DGS, MMH, AHF, SPL, SD, OD consulted for electrode design and deployment system, and performed surgery. CHC, CW, and JV wrote the initial manuscript. GC and JV secured funds for this project.

Competing interests: Parts of the technology described here are patent pending under 'Electroencephalography (EEG) Electrode Arrays and Related Methods of Use' U.S. Patent Application # PCT/US2020/051400. F. Solzbacher declares financial interest in Blackrock Microsystems LLC and Sentiomed, Inc, managed by University of Utah's COI management. W. Doyle and D. Friedman declare financial interest in Neuroview Technology overseen by NYU Grossman School of Medicine's COI management.

ORCID iDs

Chia-Han Chiang <https://orcid.org/0000-0002-4010-1266>

Charles Wang <https://orcid.org/0000-0002-2283-0529>

Katrina Barth <https://orcid.org/0000-0002-0193-5057>

Shervin Rahimpour <https://orcid.org/0000-0003-2718-181X>

Michael Trumpis <https://orcid.org/0000-0002-3834-4437>

Suseendrakumar Duraivel <https://orcid.org/0000-0002-1110-1021>

Iakov Rachinskiy <https://orcid.org/0000-0002-0087-5128>

Agrita Dubey <https://orcid.org/0000-0002-2239-9177>

Brinnae Bent <https://orcid.org/0000-0002-7039-0177>

Daniel Friedman <https://orcid.org/0000-0003-1068-1797>

Christopher F Reiche <https://orcid.org/0000-0001-6216-5888>

Derek G Southwell <https://orcid.org/0000-0001-6465-3869>

Sasha Devore <https://orcid.org/0000-0003-2554-1850>

Orrin Devinsky <https://orcid.org/0000-0003-0044-4632>

Florian Solzbacher <https://orcid.org/0000-0002-8309-9610>

Bijan Pesaran <https://orcid.org/0000-0003-4116-0038>

Gregory Cogan <https://orcid.org/0000-0003-1557-6507>

Jonathan Viventi <https://orcid.org/0000-0001-6054-0541>

References

- [1] Bergey G K *et al* 2015 Long-term treatment with responsive brain stimulation in adults with refractory partial seizures *Neurology* **84** 810–7
- [2] Benabid A L *et al* 2019 An exoskeleton controlled by an epidural wireless brain-machine interface in a tetraplegic patient: a proof-of-concept demonstration *Lancet Neurol.* **18** 1112–22
- [3] Shokoueinejad M *et al* 2019 Progress in the field of micro-electrocorticography *Micromachines* **10** 62
- [4] Brodnick S K *et al* 2019 μ ECOG recordings through a thinned skull *Front. Neurosci.* **13** 1017
- [5] Slutsky M W, Jordan L R, Krieg T, Chen M, Mogul D J and Miller L E 2010 Optimal spacing of surface electrode arrays for brain-machine interface applications *J. Neural. Eng.* **7** 26004
- [6] Welle E J, Patel P R, Woods J E, Petrossians A, Della Valle E, Vega-Medina A, Richie J M, Cai D, Weiland J D and Chestek C A 2020 Ultra-small carbon fiber electrode recording site optimization and improved *in vivo* chronic recording yield *J. Neural. Eng.* **17** 26037
- [7] Viventi J *et al* 2011 Flexible, foldable, actively multiplexed, high-density electrode array for mapping brain activity *in vivo* *Nat. Neurosci.* **14** 1599–605
- [8] Khodagholy D, Gelinas J N, Thesen T, Doyle W, Devinsky O, Malliaras G G and Buzsáki G 2014 NeuroGrid: recording action potentials from the surface of the brain *Nat. Neurosci.* **18** 310–5
- [9] Arzimanoglou A and Kahane P 2008 *Textbook of Epilepsy Surgery* 1 editor, H Luders The Ictal Onset Zone: General Principles, Pitfalls and Caveats (London: CRC Press) ch 67

pp 595–602 (<https://www.taylorfrancis.com/books/edit/10.3109/9780203091708/textbook-epilepsy-surgery-hans-luders>)

- [10] Basu I, Kudela P, Korzeniewska A, Franaszczuk P J and Anderson W S 2015 A study of the dynamics of seizure propagation across micro domains in the vicinity of the seizure onset zone *J. Neural. Eng.* **12** 046016
- [11] Kellis S, Sorensen L, Darvas F, Sayres C, O'Neill K, Brown R B, House P, Ojemann J and Greger B 2016 Multi-scale analysis of neural activity in humans: implications for micro-scale electrocorticography *Clin. Neurophysiol.* **127** 591–601
- [12] Staba R J, Stead M and Worrell G A 2014 Electrophysiological biomarkers of epilepsy *Neurotherapeutics* **11** 334–46
- [13] Stead M, Bower M, Brinkmann B H, Lee K, Marsh W R, Meyer F B, Litt B, van Gompel J and Worrell G A 2010 Microseizures and the spatiotemporal scales of human partial epilepsy *Brain* **133** 2789–97
- [14] Ray S, Crone N E, Niebur E, Franaszczuk P J and Hsiao S S 2008 Neural correlates of high-gamma oscillations (60–200 Hz) in macaque local field potentials and their potential implications in electrocorticography *J. Neurosci.* **28** 11526–36
- [15] Worrell G A, Gardner A B, Stead S M, Hu S, Goerss S, Cascino G J, Meyer F B, Marsh R and Litt B 2008 High-frequency oscillations in human temporal lobe: simultaneous microwire and clinical macroelectrode recordings *Brain* **131** 928–37
- [16] Le Van Quyen M, Staba R, Bragin A, Dickson C, Valderrama M, Fried I and Engel J 2010 Large-scale microelectrode recordings of high-frequency gamma oscillations in human cortex during sleep *J. Neurosci.* **30** 7770–82
- [17] Schevon C A, Trevelyan A J, Schroeder C E, Goodman R R, McKhann G and Emerson R G 2009 Spatial characterization of interictal high frequency oscillations in epileptic neocortex *Brain* **132** 3047–59
- [18] Dudek F E 2009 Microseizures in human neocortex: a role for ultra-small seizures? *Epilepsy Curr.* **9** 151–2
- [19] Schevon C A, Ng S K, Cappell J, Goodman R R, McKhann G, Waziri A, Branner A, Sosunov A, Schroeder C E and Emerson R G 2008 Microphysiology of epileptiform activity in human neocortex *J. Clin. Neurophysiol.* **25** 321–30
- [20] Osorio I and Frei M 2010 Feasibility of automated warning in subjects with localization-related epilepsies *Epilepsy Behav.* **19** 602–7
- [21] Cook M J et al 2013 Prediction of seizure likelihood with a long-term, implanted seizure advisory system in patients with drug-resistant epilepsy: a first-in-man study *Lancet Neurol.* **12** 563–71
- [22] Muller L, Hamilton L S, Edwards E, Bouchard K E and Chang E F 2016 Spatial resolution dependence on spectral frequency in human speech cortex electrocorticography *J. Neural. Eng.* **13** 056013
- [23] Wang W et al 2009 Human motor cortical activity recorded with Micro-ECoG electrodes, during individual finger movements *Proc 31st Annu Int Conf IEEE Eng Med Biol Soc Eng Futur Biomed EMBC 2009* pp 586–9
- [24] Leuthardt E C, Schalk G, Roland J, Rouse A and Moran D W 2009 Evolution of brain-computer interfaces: going beyond classic motor physiology *Neurosurg. Focus* **27** E4
- [25] Rouse A G, Williams J J, Wheeler J J and Moran D W 2016 Spatial co-adaptation of cortical control columns in a micro-ECoG brain–computer interface *J. Neural. Eng.* **13** 056018
- [26] Flint R D, Rosenow J M, Tate M C and Slutsky M W 2017 Continuous decoding of human grasp kinematics using epidural and subdural signals *J. Neural. Eng.* **14** 1–11
- [27] Stacey W C, Kellis S, Greger B, Butson C R, Patel P R, Assaf T, Mihaylova T and Glynn S 2013 Potential for unreliable interpretation of EEG recorded with microelectrodes *Epilepsia* **54** 1391–401
- [28] American Electroencephalographic Society 1994 Guideline twelve: guidelines for long-term monitoring for epilepsy *J. Clin. Neurophysiol.* **11** 88–110
- [29] Stacey W C, Kellis S, Patel P R, Greger B and Butson C R 2012 Signal distortion from microelectrodes in clinical EEG acquisition systems *J. Neural. Eng.* **9** 56007
- [30] Ad-Tech Medical Instrument Corporation 2008 *Epilepsy and neurosurgery product guide*
- [31] PMT Corporation 2011 *CORTAC® GRIDS & STRIPS 2011*
- [32] Woods V, Trampis M, Bent B, Palopoli-Trojani K, Chiang C H, Wang C, Yu C, Insanally M N M, Froemke R C and Viventi J 2018 Long-term recording reliability of liquid crystal polymer μ ECoG arrays *J. Neural. Eng.* **15** 066024
- [33] Orsborn A L, Wang C, Chiang K, Mahabirz M M, Viventi J and Pesaran B 2015 Semi-chronic chamber system for simultaneous subdural electrocorticography, local field potentials, and spike recordings *2015 7th Int IEEE/EMBS Conf Neural Eng. 2015* pp 398–401
- [34] Jeong J, Hyun Bae S, Seo J M, Chung H and June Kim S 2016 Long-term evaluation of a liquid crystal polymer (LCP)-based retinal prosthesis *J. Neural. Eng.* **13** 025004
- [35] Culbertson E C 1995 New laminate material for high performance PCBs: liquid crystal polymer copper clad films *Proc—Electron Components Technol Conf. 1995* pp 520–3
- [36] Palopoli-trojani K, Woods V, Chiang C H C, Trampis M and Viventi J 2016 In vitro assessment of long-term reliability of low-cost μ ECoG arrays *2016 38th Annu Int Conf IEEE Eng Med Biol Soc.* pp 4503–6
- [37] Woodward B 2012 Palladium in temporary and permanently implantable medical devices *Platin. Met. Rev.* **56** 213–7
- [38] Schulze D, Tolke R and Widmann I 2014 Noble metal PCB manufacturing for direct implants *pcb Mag.* (<https://iconnect007.com/mags/pdf.php?id=155>)
- [39] Bae S H et al 2012 *In vitro* biocompatibility of various polymer-based microelectrode arrays for retinal prosthesis *Investigative Ophthalmol. Visual Sci.* **53** 2653–7
- [40] Micro Systems Technologies DYCONEX AG. *dyconex liquid crystal polymer (lcp) substrate proves cytotoxicity conformity according to iso 10993–5*
- [41] Petrossians A, Whalen J J, Weiland J D and Mansfeld F 2011 Surface modification of neural stimulating/recording electrodes with high surface area platinum-iridium alloy coatings *Proc Annu Int Conf IEEE Eng Med Biol Soc EMBS 2011* pp 3001–4
- [42] Petrossians A, Davuluri N, Whalen J J, Mansfeld F and Weiland J D 2014 Improved biphasic pulsing power efficiency with Pt-Ir coated microelectrodes *MRS Proc. 1621: mrsf13-1621-j07-03 1621 249–57*
- [43] Cassar I R, Yu C, Sambangi J, Lee C D, Whalen J J, Petrossians A and Grill W M 2019 Electrodeposited platinum-iridium coating improves *in vivo* recording performance of chronically implanted microelectrode arrays *Biomaterials* **205** 120–32
- [44] Wagoner T 2017 *Samtec ZA8 Extended Life Test Report 2017* (<https://doi.org/10.1111/jtxs.12298>)
- [45] Arieli A, Grinvald A and Slovin H 2002 Dural substitute for long-term imaging of cortical activity in behaving monkeys and its clinical implications *J. Neurosci. Methods* **114** 119–33
- [46] Ruiz O, Lustig B R, Nassi J J, Cetin A, Reynolds J H, Albright T D, Callaway E M, Stoner G R and Roe A W 2013 Optogenetics through windows on the brain in the nonhuman primate *J. Neurophysiol.* **110** 1455–67
- [47] Chiang C H, Lee J, Wang C, Williams A J, Lucas T H, Cohen Y E and Viventi J 2020 A modular high-density μ ECoG system on macaque vLPFC for auditory cognitive decoding *J. Neural. Eng.* **17** 046008
- [48] Witham N S et al 2017 *Flexural bending to approximate cortical forces exerted by electrocorticography (ECoG) arrays* *Prep.* (<https://doi.org/10.1088/1741-2552/ac02dc>)
- [49] Trampis M, Chiang C H, Orsborn A L, Bent B, Li J, Rogers J A, Pesaran B, Cogan G and Viventi J 2020 Sufficient sampling for kriging prediction of cortical potential in rat, monkey, and human μ ECoG *J. Neural Eng.* **18** 036011

[50] Cogan G B, Iyer A, Melloni L, Thesen T, Friedman D, Doyle W, Devinsky O and Pesaran B 2017 Manipulating stored phonological input during verbal working memory *Nat. Neurosci.* **20** 279–86

[51] Canolty R T, Edwards E, Dalal S S, Soltani M, Nagarajan S S, Kirsch H E, Berger M S, Barbaro N M and Knight R T 2006 High gamma power is phase-locked to theta oscillations in human neocortex *Source Sci. New Ser.* **313** 1626–8

[52] Miller K J, Zanos S, Fetz E E, Den Nijs M and Ojemann J G 2009 Decoupling the cortical power spectrum reveals real-time representation of individual finger movements in humans *J. Neurosci.* **29** 3132–7

[53] Crone N E, Boatman D, Gordon B and Hao L 2001 Induced electrocorticographic gamma activity during auditory perception *Clin. Neurophysiol.* **112** 565–82

[54] Akbari H, Khalighinejad B, Herrero J, Mehta A and Mesgarani N 2019 Towards reconstructing intelligible speech from the human auditory cortex *Sci. Rep.* **9** 874

[55] Cogan G B, Thesen T, Carlson C, Doyle W, Devinsky O and Pesaran B 2014 Sensory–motor transformations for speech occur bilaterally *Nature* **507** 94–98

[56] Benjamini Y and Hochberg Y 1995 Controlling the false discovery rate: a practical and powerful approach to multiple testing *J. R. Stat. Soc. B* **57** 289–300

[57] Insanally M, Trumppi M, Wang C, Chiang C-H, Woods V, Palopoli-Trojani K, Bossi S, Froemke R C and Viventi J 2016 A low-cost, multiplexed μ ECoG system for high-density recordings in freely moving rodents *J. Neural. Eng.* **13** 026030

[58] Duraivel S, Rao A T, Lu C W, Bentley J N, Stacey W C, Chestek C A and Patil P G 2020 Comparison of signal decomposition techniques for analysis of human cortical signals *J. Neural. Eng.* **17** 056014

[59] Cogan S F, Ludwig K A, Welle C G and Takmakov P 2016 Tissue damage thresholds during therapeutic electrical stimulation *J. Neural. Eng.* **13** 021001

[60] Takemi M, Castagnola E, Ansaldi A, Ricci D, Fadiga L, Taoka M, Iriki A and Ushiba J 2017 Rapid identification of cortical motor areas in rodents by high-frequency automatic cortical stimulation and novel motor threshold algorithm *Front. Neurosci.* **11** 580

[61] Lu Y, Lyu H, Richardson A G, Lucas T H and Kuzum D 2016 Flexible neural electrode array based-on porous graphene for cortical microstimulation and sensing *Sci. Rep.* **6** 1–9

[62] Vaskov A K, Irwin Z T, Nason S R, Vu P P, Nu C S, Bullard A J, Hill M, North N, Patil P G and Chestek C A 2018 Cortical decoding of individual finger group motions using ReFIT kalman filter *Front. Neurosci.* **12** 751

[63] Tandon N, Tong B A, Friedman E R, Johnson J A, Von Allmen G, Thomas M S, Hope O A, Kalamangalam G P, Slater J D and Thompson S A 2019 Analysis of morbidity and outcomes associated with use of subdural grids vs stereoelectroencephalography in patients with intractable epilepsy *JAMA Neurol.* **76** 672

[64] Pothof F, Bonini L, Lanzilotto M, Livi A, Fogassi L, Orban G A, Paul O and Ruther P 2016 Chronic neural probe for simultaneous recording of single-unit, multi-unit, and local field potential activity from multiple brain sites *J. Neural. Eng.* **13** 046006

[65] Cressie N 1990 The origins of kriging *Math. Geol.* **22** 239–52

[66] Musk E 2019 An integrated brain-machine interface platform with thousands of channels *J. Med. Internet Res.* **21** e16194

[67] Jun J J *et al* 2017 Fully integrated silicon probes for high-density recording of neural activity *Nature* **551** 232–6

[68] Chiang C H *et al* 2020 Development of a neural interface for high-definition, long-term recording in rodents and nonhuman primates *Sci. Transl. Med.* **12** eaay4682

[69] Worrell G A, Jerbi K, Kobayashi K, Lina J M, Zelmann R and Le Van Quyen M 2012 Recording and analysis techniques for high-frequency oscillations *Prog. Neurobiol.* **98** 265–78

[70] Wiebe S, Blume W T, Girvin J P and Eliasziw M 2001 A randomized, controlled trial of surgery for temporal-lobe epilepsy *New Engl. J. Med.* **345** 311–8

[71] Wetjen N M, Marsh W R, Meyer F B, Cascino G D, So E, Britton J W, Stead S M and Worrell G A 2009 Intracranial electroencephalography seizure onset patterns and surgical outcomes in nonlesional extratemporal epilepsy *J. Neurosurg.* **110** 1147–52

[72] Blanco J A *et al* 2011 Data mining neocortical high-frequency oscillations in epilepsy and controls *Brain* **134** 2948–59

[73] Tarulli A, Devinsky O and Alper K 2001 Progression of postictal to interictal psychosis *Epilepsia* **42** 1468–71

[74] Beauchamp M S, Oswalt D, Sun P, Foster B L, Magnotti J F, Niketeghad S, Pouratian N, Bosking W H and Yoshor D 2020 Dynamic stimulation of visual cortex produces form vision in sighted and blind humans *Cell* **181** 774–783.e5

[75] Miller K J, Leuthardt E C, Schalk G, Rao R P N, Anderson N R, Moran D W, Miller J W and Ojemann J G 2007 Spectral changes in cortical surface potentials during motor movement *J. Neurosci.* **27** 2424–32

[76] Mehring C, Rickert J, Vaadia E, Cardosa De Oliveira S, Aertsen A and Rotter S 2003 Inference of hand movements from local field potentials in monkey motor cortex *Nat. Neurosci.* **6** 1253–4

[77] Thongpang S *et al* 2011 A micro-electrocorticography platform and deployment strategies for chronic BCI applications *Clin. EEG Neurosci.* **42** 259–65

[78] Kellis S, Miller K, Thomson K, Brown R, House P and Greger B 2010 Decoding spoken words using local field potentials recorded from the cortical surface *J. Neural. Eng.* **7** 056007

[79] Kellis S S, House P A, Thomson K E, Brown R and Greger B 2009 Human neocortical electrical activity recorded on nonpenetrating microwire arrays: applicability for neuroprostheses *Neurosurg. Focus* **27** E9

[80] Middlebrooks J C, Bierer J A and Snyder R L 2005 Cochlear implants: the view from the brain *Curr. Opin. Neurobiol.* **15** 488–93

[81] Froemke R C, Heman-Ackah S and Waltzman S 2014 *Cochlear Implant* 3rd edn editors S Waltzman and J T Roland Auditory Neuroplasticity (Thieme) **4** 38–46

[82] Rao V R, Sellers K K, Wallace D L, Lee M B, Bijanzadeh M, Sani O G, Yang Y, Shanechi M M, Dawes H E and Chang E F 2018 Direct electrical stimulation of lateral orbitofrontal cortex acutely improves mood in individuals with symptoms of depression *Curr. Biol.* **28** 3893–3902.e4

[83] Sani O G, Yang Y, Lee M B, Dawes H E, Chang E F and Shanechi M M 2018 Mood variations decoded from multi-site intracranial human brain activity *Nat. Biotechnol.* **36** 954

[84] Milekovic T *et al* 2018 Stable long-term BCI-enabled communication in ALS and locked-in syndrome using LFP signals *J. Neurophysiol.* **120** 343–60

[85] Baud M O, Kleen J K, Anumanchipalli G K, Hamilton L S, Tan Y L, Knowlton R and Chang E F 2018 Unsupervised learning of spatiotemporal interictal discharges in focal epilepsy *Neurosurgery* **83** 683–91

[86] Gliske S V, Irwin Z T, Chestek C, Hegeman G L, Brinkmann B, Sagher O, Garton H J L, Worrell G A and Stacey W C 2018 Variability in the location of high frequency oscillations during prolonged intracranial EEG recordings *Nat. Commun.* **9** 2155