

Computational investigation of left ventricular hemodynamics following bioprosthetic aortic and mitral valve replacement

Fei Xu^a, Emily L. Johnson^b, Chenglong Wang^c, Arian Jafari^b, Cheng-Hau Yang^b, Michael S. Sacks^{d,e}, Adarsh Krishnamurthy^b, Ming-Chen Hsu^{b,*}

^a Ansys Inc., Austin, TX 78746, USA

^b Department of Mechanical Engineering, Iowa State University, Ames, IA 50011, USA

^c Ansys Inc., Lebanon, NH 03766, USA

^d Oden Institute for Computational Engineering and Sciences, The University of Texas at Austin, Austin, TX 78712, USA

^e Department of Biomedical Engineering, The University of Texas at Austin, Austin, TX 78712, USA

ARTICLE INFO

Article history:

Received 27 February 2020

Revised 17 August 2020

Accepted 17 September 2020

Available online 16 October 2020

Keywords:

Fluid–structure interaction

Immersogeometric analysis

Cardiac biomechanics and hemodynamics

Bioprosthetic heart valves

Aortic and mitral valve replacement

ABSTRACT

The left ventricle of the heart is a fundamental structure in the human cardiac system that pumps oxygenated blood into the systemic circulation. Several valvular conditions can cause the aortic and mitral valves associated with the left ventricle to become severely diseased and require replacement. However, the clinical outcomes of such operations, specifically the postoperative ventricular hemodynamics of replacing both valves, are not well understood. This work uses computational fluid–structure interaction (FSI) to develop an improved understanding of this effect by modeling a left ventricle with the aortic and mitral valves replaced with bioprostheses. We use a hybrid Arbitrary Lagrangian–Eulerian/immersogeometric framework to accommodate the analysis of cardiac hemodynamics and heart valve structural mechanics in a moving fluid domain. The motion of the endocardium is obtained from a cardiac biomechanics simulation and provided as an input to the proposed numerical framework. The results from the simulations in this work indicate that the replacement of the native mitral valve with a tri-radially symmetric bioprosthesis dramatically changes the ventricular hemodynamics. Most significantly, the vortical motion in the left ventricle is found to reverse direction after mitral valve replacement. This study demonstrates that the proposed computational FSI framework is capable of simulating complex multiphysics problems and can provide an in-depth understanding of the cardiac mechanics.

© 2020 Elsevier Ltd. All rights reserved.

1. Introduction

In the cardiac system, the left ventricle (LV) is responsible for receiving oxygenated blood from the left atrium (LA) and pumping it into the human systemic circulation. The two heart valves associated with the LV, the aortic valve (AV) and the mitral valve (MV), work in coordination to ensure unidirectional flow through the cardiac system. On the left side of the heart, the higher pressure and associated increases in cyclic loading make the AV and MV more susceptible to cardiac diseases than the valves on the right side of the heart [1]. Valvular heart diseases [2] can severely deteriorate the normal function of these valves and fundamentally disrupt the cardiac hemodynamics. For patients with severe valvular diseases, heart valve replacement is one of the most viable intervention options, resulting in around 75,000 prosthetic

implants in the United States and around 170,000 to 250,000 implants in the world annually [3,4]. Recently, surgical bioprosthetic heart valves (BHVs), which are tri-radially symmetric devices that are designed to mimic the anatomy of the AV, have become the predominant choice for valve replacement operations [5]. Although the anatomies of the AV and MV are entirely different, it is a common practice to use the same BHV design (e.g. Medtronic Mosaic valve [6]) for both aortic and mitral valve replacements [7]. While the asymmetry of the native MV is believed to result in a circulatory flow pattern in the LV that aids in the washout of ventricular blood during systole [8,9], the replacement of the native MV with a symmetric BHV may alter this flow pattern and negatively influence the cardiac hemodynamics [10,11]. Furthermore, the clinical outcomes after combined aortic and mitral valve surgery are not well known [12]. In an effort to develop an improved understanding of these effects, this work proposes a computational fluid–structure interaction (FSI) framework for the simulation of the LV with both the AV and MV replaced with surgical BHVs.

* Corresponding author.

E-mail address: jmchsu@iastate.edu (M.-C. Hsu).

The simulation of the intricate structures and function of the cardiac system requires suitable modeling and analysis methods that can accurately capture the physical complexity of this system. However, most of the previous LV simulations have utilized simplified assumptions regarding the LV geometry, deformation, or boundary conditions [13–16], which significantly reduce the feasibility of effectively replicating the in-vivo cardiac motions or hemodynamics. In recent years, vascular simulations (i.e. simulations of blood flows inside the vessels connected to the heart) have reached a relatively mature state [17–21] with even clinical applications [22–25]. At the same time, cardiac hemodynamics simulations (i.e. simulations of blood flows in the four chambers of the heart) still face many challenges, despite the advancements that have been made over the last decade [26–30]. Some of these challenges include obtaining the time-dependent large-scale heart-chamber deformation, resolving the complex hemodynamics, and considering their interactions with the structural mechanics of the heart valves [31]. As a result, realistic and robust numerical modeling of the cardiac system requires advanced FSI formulations and methodologies.

To approach the computational challenges of this complex system, traditional boundary-fitted methods for moving domain simulations, including the Arbitrary Lagrangian–Eulerian (ALE) [32–34] and Space–Time (ST) [35–37] methods, have been successfully applied to modeling the hemodynamics of wall-bounded biomedical problems [38–42]. However, for simulations that consider the geometries and motions of the heart valves, the large structural deformation of the valve leaflets can severely distort the boundary-fitted fluid elements if they are continuously deformed from a single reference configuration of the computational domain. Sophisticated mesh management algorithms are often required [43–45] to handle this type of problem. In addition, the heart valve experiences contact between the leaflets. Some existing specialized contact algorithms either impose a small distance to separate surfaces that would otherwise come into contact [46] or prescribe locations where the contact would occur [30,47,48]. While these assumptions are often sufficient for some idealized scenarios, they are inadequate for general valvular FSI simulations.

In light of these limitations for cardiac applications, immersogeometric analysis (IMGA) [49] was proposed as a geometrically flexible method to model and simulate heart valve FSI problems [50–54]. This novel method makes direct use of the CAD boundary representation (B-rep) of a complex design structure by immersing it into a non-boundary-fitted discretization of the surrounding fluid domain [55–59]. This approach effectively deals with FSI problems involving structures with complex motion that leads to large deformations of the fluid domain, including changes of topology [60,61]. Algorithms developed for structural contact and impact problems [62,63] can also be directly adopted in the IMGA simulations. The variational formulation for immersogeometric FSI analysis was derived using a dynamic augmented Lagrangian (DAL) approach to weakly enforce kinematic and traction constraints [64,65]. A hybrid ALE/IMGA methodology, in which a single computation combines both a boundary-fitted, deforming-mesh treatment of some fluid–structure interfaces and a non-boundary-fitted treatment of others, was also developed under the same framework [50]. A comprehensive review of IMGA and its recent developments and applications in heart valve simulations can be found in Hsu and Kamensky [66].

In this work, based on the different types of deformation present in the LV and BHV subproblems, we formulate an FSI framework in which the LV is treated with a boundary-fitted, deforming-mesh ALE approach and the BHVs are treated with a non-boundary-fitted IMGA approach. Within this hybrid ALE/IMGA concept, a variety of advanced technologies are seamlessly integrated, including geometry modeling [67], fluid dynamics [68],

structural mechanics [69,70], and structural contact/impact [71]. Such a versatile technology is well suited for the multiscale, multiphysics modeling environment of cardiac flows. The detailed geometry and deformation information for the LV are obtained over the complete cardiac cycle from a separate cardiac biomechanics simulation, which is based on the technology proposed in Krishnamurthy et al. [72], and used as an input to the cardiac FSI simulation. A high-quality fluid domain finite element mesh is created and deformed in time in a boundary-fitted fashion following the endocardial surface information obtained from the biomechanics simulation of the LV. Using the corresponding annulus information, we construct two BHVs, one attached to the aortic annulus and one to the mitral annulus, and immerse them into the background LV fluid meshes. These two distinct approaches are integrated within our hybrid ALE/IMGA framework to solve for the complex hemodynamics of the LV coupled to the structural mechanics of the BHVs. Particular emphasis is placed on understanding the alteration in the left ventricular hemodynamic pattern that may result from these valve replacements.

This paper is organized as follows. In Section 2, we present the main constituents of the hybrid ALE/IMGA framework for solving the cardiac and valvular FSI problem. Section 3 details the techniques for obtaining the LV geometry and its time-dependent motion over a complete cardiac cycle, and the problem setup of the ventricular FSI simulation. The results are presented in Section 4, in which we demonstrate and discuss the LV flow pattern after bioprosthetic aortic and mitral valve replacement. Finally, we draw conclusion and motivate future research in Section 5.

2. Fluid–structure interaction methodology

In this section, we present the main constituents of the hybrid ALE/IMGA FSI framework for simulating cardiac problems. We start with the discussion of the DAL FSI framework. We then provide a comprehensive overview on the numerical formulations for all the subproblems in the FSI system. Finally, we demonstrate how the numerical ingredients are integrated together within the ALE/IMGA framework.

2.1. Mathematical model of the FSI problem

The LV FSI problem is governed by a partial differential equation (PDE) system, described using the augmented Lagrangian framework, that consists of the fluid subproblem, the structure subproblem, and a Lagrange multiplier constraint problem to enforce the compatibility of kinematics and tractions at the fluid–structure interface [49,66,73]. For a thin structure Γ_t in a fluid domain Ω_t , the FSI problem can be expressed as: Find a fluid velocity $\mathbf{u}_1 \in S_u$ and fluid pressure $p \in S_p$, a structure displacement $\mathbf{y} \in S_y$ with its material time derivative denoted as $\mathbf{u}_2$, and a Lagrange multiplier $\boldsymbol{\lambda} \in S_\ell$ such that for all test functions $\mathbf{w}_1 \in \mathcal{V}_u$, $q \in S_q$, $\mathbf{w}_2 \in \mathcal{V}_y$, and $\delta \boldsymbol{\lambda} \in \mathcal{V}_\ell$,

$$\begin{aligned} B_1(\{\mathbf{w}_1, q\}, \{\mathbf{u}_1, p\}) - F_1(\{\mathbf{w}_1, q\}) + B_2(\mathbf{w}_2, \mathbf{y}) - F_2(\mathbf{w}_2) \\ + \int_{\Gamma_t} (\mathbf{w}_1 - \mathbf{w}_2) \cdot \boldsymbol{\lambda} \, d\Gamma + \int_{\Gamma_t} \delta \boldsymbol{\lambda} \cdot (\mathbf{u}_1 - \mathbf{u}_2) \, d\Gamma \\ + \int_{\Gamma_t} (\mathbf{w}_1 - \mathbf{w}_2) \cdot \beta (\mathbf{u}_1 - \mathbf{u}_2) \, d\Gamma = 0, \end{aligned} \quad (1)$$

where $S_{(\cdot)}$ and $\mathcal{V}_{(\cdot)}$ are trial solution and test function spaces, $B(\cdot, \cdot)$ and $F(\cdot)$ are functionals defining the fluid and structure subproblems, denoted by subscript 1 and 2 respectively, and β is a penalty parameter that enforces the compatibility of kinematics on the immersed thin structure. The presence of the Lagrange multiplier and penalty terms facilitates the development of certain numerical schemes based on the “augmented Lagrangian” concept [73],

as it is valid regardless of matching or non-matching discretizations at the fluid–structure interface. For this reason, although the augmented Lagrangian framework was originally developed for boundary-fitted simulations, it can be straightforwardly applied to the context of immersed interface problems.

Remark 1. If the fluid and structural velocities and the corresponding test functions are explicitly assumed to be continuous (i.e., $\mathbf{u}_1 = \mathbf{u}_2$ and $\mathbf{w}_1 = \mathbf{w}_2$) at the interface, the second and third lines of Eq. (1) drop out and the FSI formulation of Eq. (1) reduces to a form suitable for matching fluid–structure interface meshes.

2.2. Hemodynamics

The fluid subproblem (hemodynamics) is governed by the Navier–Stokes equations of incompressible flows on a moving domain. The ALE formulation is adopted to account for the motion of the deforming LV, which is tracked by a boundary-fitted mesh that morphs with it. Advanced mesh moving techniques [74–76] are used to preserve the mesh quality throughout the entire cardiac cycle. The advantage of the ALE formulation is that the kinematic constraints on the boundaries are naturally satisfied by construction. The ALE formulation has been proven effective in a variety of vascular flow simulations [77,78], for which comprehensive reviews can be found in Takizawa et al. [79].

The ALE form of the Navier–Stokes equations is discretized using a variational multiscale (VMS) approach [68,80–84], in which the stabilization parameter is modified to improve the conservation of mass in the presence of an immersed thin structure [64]. We introduce a collection of disjoint fluid elements $\{\Omega^e\}$ such that $\Omega = \cup_e \Omega^e$, and replace the semi-linear form B_1 and linear functional F_1 in Eq. (1) with their ALE-VMS counterparts, which take the forms of

$$\begin{aligned} B_1^{\text{VMS}}(\{\mathbf{w}_1, q\}, \{\mathbf{u}_1, p\}) &= \int_{\Omega_t} \mathbf{w}_1 \cdot \rho_1 \left(\frac{\partial \mathbf{u}_1}{\partial t} \Big|_{\bar{\mathbf{x}}} + (\mathbf{u}_1 - \hat{\mathbf{u}}) \cdot \nabla \mathbf{u}_1 \right) d\Omega \\ &+ \int_{\Omega_t} \boldsymbol{\varepsilon}(\mathbf{w}_1) : \boldsymbol{\sigma}_1 d\Omega + \int_{\Omega_t} q \nabla \cdot \mathbf{u}_1 d\Omega \\ &- \sum_e \int_{\Omega_t^e} \left((\mathbf{u}_1 - \hat{\mathbf{u}}) \cdot \nabla \mathbf{w}_1 + \frac{\nabla q}{\rho_1} \right) \cdot \mathbf{u}_1' d\Omega \\ &- \sum_e \int_{\Omega_t^e} p' \nabla \cdot \mathbf{w}_1 d\Omega \\ &+ \sum_e \int_{\Omega_t^e} \mathbf{w}_1 \cdot (\mathbf{u}_1' \cdot \nabla \mathbf{u}_1) d\Omega \\ &- \sum_e \int_{\Omega_t^e} \frac{\nabla \mathbf{w}_1}{\rho_1} : (\mathbf{u}_1' \otimes \mathbf{u}_1') d\Omega \\ &+ \sum_e \int_{\Omega_t^e} (\mathbf{u}_1' \cdot \nabla \mathbf{w}_1) \bar{\tau} \cdot (\mathbf{u}_1' \cdot \nabla \mathbf{u}_1) d\Omega, \end{aligned} \quad (2)$$

and

$$F_1^{\text{VMS}}(\{\mathbf{w}_1, q\}) = \int_{\Omega_t} \mathbf{w}_1 \cdot \rho_1 \mathbf{f}_1 d\Omega + \int_{(\Gamma_h)_t} \mathbf{w}_1 \cdot \mathbf{h}_1 d\Gamma, \quad (3)$$

where ρ_1 is the fluid mass density, $\boldsymbol{\varepsilon}$ is the symmetric gradient operator, $\boldsymbol{\sigma}_1(\mathbf{u}_1, p) = -p\mathbf{I} + 2\mu\boldsymbol{\varepsilon}(\mathbf{u}_1)$, where μ is the dynamic viscosity, $\mathbf{f}_1$ is a prescribed body force, $\mathbf{h}_1$ is a prescribed traction on $\Gamma_h \subset \partial\Omega$, $\partial(\cdot)/\partial t|_{\bar{\mathbf{x}}}$ indicates time differentiation with respect to a fixed point $\bar{\mathbf{x}}$ from some reference configuration Ω_0 , $\mathbf{u}_1'$ is the fine scale velocity ansatz,

$$\mathbf{u}_1' = -\tau_M \left(\rho_1 \left(\frac{\partial \mathbf{u}_1}{\partial t} \Big|_{\bar{\mathbf{x}}} + (\mathbf{u}_1 - \hat{\mathbf{u}}) \cdot \nabla \mathbf{u}_1 - \mathbf{f}_1 \right) - \nabla \cdot \boldsymbol{\sigma}_1 \right), \quad (4)$$

p' is the fine scale pressure,

$$p' = -\rho_1 \tau_C \nabla \cdot \mathbf{u}_1, \quad (5)$$

and the mesh $\{\Omega^e\}$ deforms with velocity $\hat{\mathbf{u}}$. The detailed definition of the stabilization parameters τ_M , τ_C , and $\bar{\tau}$ can be found in Kamensky et al. [64]. The first three terms of the right hand side of Eq. (2) correspond to the standard Galerkin form of the Navier–Stokes equations, and the rest of the terms are the VMS entries, which can be interpreted both as a stabilized formulation and a large-eddy simulation (LES) turbulence model [68,85–89].

Finally, the formulation of the fluid subproblem is enhanced by a weakly enforced no-slip boundary condition operator on the LV surface. Let $(\Gamma_D)_t \in \Gamma_t$ be the part of the boundary where Dirichlet velocity boundary conditions are applied. We replace the traditional strong enforcement of Dirichlet boundary conditions by adding the following weak-boundary-condition operator to the left hand side of the fluid subproblem:

$$\begin{aligned} &- \int_{(\Gamma_D)_t} \mathbf{w}_1 \cdot (-p\mathbf{n} + 2\mu\boldsymbol{\varepsilon}(\mathbf{u}_1)\mathbf{n}) d\Gamma \\ &- \int_{(\Gamma_D)_t} (2\mu\boldsymbol{\varepsilon}(\mathbf{w}_1)\mathbf{n} + q\mathbf{n}) \cdot (\mathbf{u}_1 - \mathbf{g}) d\Gamma \\ &- \int_{(\Gamma_D^-)_t} \mathbf{w}_1 \cdot \rho_1 ((\mathbf{u}_1 - \hat{\mathbf{u}}) \cdot \mathbf{n}) (\mathbf{u}_1 - \mathbf{g}) d\Gamma \\ &+ \int_{(\Gamma_D)_t} \mathbf{w}_1 \cdot \tau^B (\mathbf{u}_1 - \mathbf{g}) d\Gamma. \end{aligned} \quad (6)$$

The first two terms of the above equation are the consistency and adjoint consistency terms, respectively [90]. The last two terms provide additional numerical stabilities and help better satisfy the no-slip and no-penetration boundary conditions by penalizing the fluid velocity $\mathbf{u}_1$ toward the prescribe velocity $\mathbf{g}$ on the Dirichlet boundary. The third term is imposed on $(\Gamma_D^-)_t$, which is the “in-flow” part of $(\Gamma_D)_t$ where $(\mathbf{u}_1 - \hat{\mathbf{u}}) \cdot \mathbf{n} < 0$. The τ^B in the fourth term is chosen element-wise as $\tau^B = 4\mu/h_n$, where h_n is the wall-normal element size at the boundary. This definition ensures the stability of the formulation, yet does not overshadow the consistency and adjoint consistency terms that are responsible for the excellent robustness and accuracy of the weak enforcement of boundary conditions. The formulation allows the flow to slip on the boundary when the fluid mesh in the boundary layer is coarse, which mimics the presence of a wall function and therefore avoids the excessive resolution requirement of the boundary-layer meshes [68,90–92].

2.3. Heart valve structure modeling

The BHV structures are modeled by an isogeometric hyperelastic thin shell formulation developed in Kiendl et al. [69]. The formulation is based on the Kirchhoff–Love assumption with an arbitrary hyperelastic constitutive model. Let $(\Gamma^{\text{sh}})_t \in \Gamma_t$ denote the midsurface of the BHVs and $(\Gamma^{\text{sh}})_0$ being its reference configuration, the semi-linear form B_2 and linear functional F_2 defining the nonlinear elasticity problem can be expressed as

$$\begin{aligned} B_2(\mathbf{w}_2, \mathbf{y}) &= \int_{(\Gamma^{\text{sh}})_t} \mathbf{w}_2 \cdot \rho_2 h_{\text{th}} \frac{\partial^2 \mathbf{y}}{\partial t} \Big|_{\mathbf{x}} d\Gamma \\ &+ \int_{(\Gamma^{\text{sh}})_0} \int_{-h_{\text{th}}/2}^{h_{\text{th}}/2} D_{\mathbf{w}_2} \mathbf{E} : \mathbf{S} d\xi^3 d\Gamma, \end{aligned} \quad (7)$$

$$F_2(\mathbf{w}_2) = \int_{(\Gamma^{\text{sh}})_t} \mathbf{w}_2 \cdot \rho_2 h_{\text{th}} \mathbf{f}_2 d\Gamma + \int_{(\Gamma^{\text{sh}})_t} \mathbf{w}_2 \cdot \mathbf{h}_2 d\Gamma, \quad (8)$$

where ρ_2 is the structure mass density, h_{th} is the shell thickness, $\partial(\cdot)/\partial t|_{\mathbf{x}}$ indicates the time derivative taken with respect to a fixed material point $\mathbf{x}$, ξ^3 is the shell through-thickness coordinate, $\mathbf{f}_2$ is

a prescribed body force, $\mathbf{h}_2$ is the net fluid traction acting on the BHV leaflets, $\mathbf{E}$ is the Green–Lagrange strain tensor depending entirely on the shell midsurface displacement $\mathbf{y}$, $D_{\mathbf{w}_2}\mathbf{E}$ is the variation of $\mathbf{E}$ in the direction $\mathbf{w}_2$, and $\mathbf{S}$ is the second Piola–Kirchhoff stress tensor. In this work, the BHV leaflets are assumed to be incompressible and are modeled as a Fung-type material. Specifically, $\mathbf{S}$ is computed as

$$\mathbf{S} = 2 \frac{\partial \psi_{el}}{\partial \mathbf{C}} - p_l \mathbf{C}^{-1}, \quad (9)$$

where

$$\psi_{el} = \frac{c_0}{2} (I_1 - 3) + \frac{c_1}{2} (e^{c_2(I_1-3)^2} - 1). \quad (10)$$

In the above equations, $\mathbf{C} = 2\mathbf{E} + \mathbf{I}$ is the left Cauchy–Green deformation tensor, p_l is a Lagrange multiplier that can be analytically determined using the plane stress condition to enforce incompressibility, $I_1 = \text{tr } \mathbf{C}$, and c_0 , c_1 , and c_2 are material parameters.

The Fung-type material model uses a combination of linear and exponential functions of the first strain invariant [93–95] to describe the tissue stiffening under tensile loading. For the small strain regimes, such as those present in the open aortic BHV configuration during LV systole, the tissue remains compliant, since the unloaded collagen fibers are highly undulated and only provide very low stiffness. The extracellular matrix dominates the material stiffness, and is modeled here by the incompressible neo-Hookean term proposed by Fan and Sacks [96]. As the strain increases, the magnitude of the exponential term begins to dominate, which mimics the drastic increase in the stiffness of stretched biological tissues, such as when the aortic BHV closes subject to the large transvalvular pressure load during LV diastole.

Remark 2. In this work, the contact between the leaflets is assumed to be frictionless and is modeled using a penalty-based approach detailed in Kamensky et al. [49], in which a repulsive force is applied to the leaflet structures that come into contact. In our hybrid ALE/IMGA framework, since the discretization of the BHVs are independent from the fluid, other existing contact algorithms may be directly incorporated. For example, the volumetric-potential-based algorithms developed by Kamensky et al. [71,97] are suitable options to model self contact and frictions.

2.4. Fluid–structure coupling

The thin-shell BHV structures described in the previous section are “immersed” into the background LV fluid mesh. The coupling between the fluid and thin shell is achieved using the IMGA approach through a combination of the penalty and the Lagrangian multiplier field shown in Eq. (1). The semi-linear forms and linear functionals in the fluid and structure subproblems are discretized in time using the generalized- α method [98]. Note that the fluid–structure interface Γ_t^{sh} is not conforming to the fluid mesh elements $\cup_e \Omega^e$. Therefore, the Lagrange multiplier field on Γ_t^{sh} needs to be approximated in the context of the non-boundary-fitted discretization. Following the DAL approach [64,66], the Lagrange multiplier is discretized in space and updated semi-implicitly in each time step. In short, in the case in which a thin shell is immersed into the fluid, the tangential component of the Lagrange multiplier is eliminated such that the non-sliding condition is only enforced by the tangential component of the penalty, β_{TAN} . The normal component $\lambda = \boldsymbol{\lambda} \cdot \mathbf{n}^{\text{sh}}$ is stored at the quadrature points of the thin shell Γ^{sh} (with $\mathbf{n}^{\text{sh}}$ being its unit outward normal vector) in the form of a scalar, and is used together with the normal penalty β_{NOR} to enforce the no-penetration conditions. λ is updated in time by

$$\lambda^{n+1} = \frac{1}{r+1} (\lambda^n + \beta_{\text{NOR}} (\mathbf{u}_1^{n+\alpha_f} - \mathbf{u}_2^{n+\alpha_f}) \cdot \mathbf{n}^{\text{sh}}), \quad (11)$$

where $n + \alpha_f$ is an intermediate time level between steps n and $n + 1$ that is predicted by the generalized- α method. The constant parameter $r \geq 0$, which is inspired by the perturbed Lagrangian approach [99], ensures well-posedness in the steady limit. Kamensky et al. [64, 100] analyzed the stability and accuracy of this methodology as well as the choices of the parameters. Following their recommendation, we set $r = 10^{-5}$ for the semi-implicit time integration scheme for Lagrange multiplier in Eq. (11).

Remark 3. The hybrid ALE/IMGA framework falls under the concept of the Fluid–Solid Interface-Tracking/Interface-Capturing Technique (FSITICT) [101]. In such a paradigm, interfaces that are feasible to track are tracked (e.g. the LV motion), and those that are too challenging to track are captured (e.g. the BHVs). In the present work, the immersion of the non-boundary-fitted BHV structures into a boundary-fitted discretization of the deforming LV is a typical example of FSITICT. The FSITICT was recently introduced to compressible flow simulations with application to rotorcraft aerodynamics [58].

3. Ventricular fluid–structure interaction simulation

In this section, we present the implementation details for simulating blood flow inside an LV model in which the native AV and MV are replaced with BHVs. Based on the LV motion obtained from a cardiac biomechanics simulation, we use an interactive geometry framework [67] to construct the fluid mesh and BHV models, and specify the boundary conditions of the FSI problem in a complete cardiac cycle.

3.1. Structural analysis of LV motion

The physiological LV wall motion used in this work is generated through a standalone structural simulation of the cardiac mechanics [70,72]. A brief summary of this technology is presented here. A biventricular cardiac model, which includes both the left and the right ventricles, orifices, and valve annuli, is constructed using cubic-Hermite finite element meshes. The model dimensions, including the volume of both ventricles and wall (myocardium) thickness, were adjusted using data from available literature [102]. Although high order smoothness can be achieved in the interior of Hermite elements, maintaining continuity of the fields across element boundaries requires additional mathematical constraints, especially at extraordinary nodes that are connected to a non-regular number of edges (3, or ≥ 5). Following the work of Krishnamurthy et al. [72], a local-to-global map [103] that transforms global ensemble derivatives into local element derivatives is used to maintain the continuity at extraordinary nodes. In addition, the accurate myocardial fiber architecture is crucial to the physiological realism of the LV structural mechanics. A coordinate frame interpolation method is developed to maintain the consistency of the fiber orientation within the elements, even in the presence of extraordinary nodes [104]. The passive material properties of the myocardial tissue are modeled by the hyperelastic constitutive model [105]. This is a nonlinear hyperelastic constitutive law for which the strain energy is an exponential function of the right Cauchy–Green strain tensor in the fiber direction and the transverse direction as separate terms. Using the three-wall segment (TriSeg) model [106], the muscle contraction is modeled as a time-dependent active stress that is added to the passive stress in the 3D finite element formulation. Finally, to obtain the deformation of the biventricular model for the complete cardiac cycle, the 3D finite element model is coupled with a lumped-parameter closed-loop circulation model that represents the rest of the cardiovascular system. For details on the setup and numerical methodologies used for the cardiac structural model, we refer the readers to the cited literature.

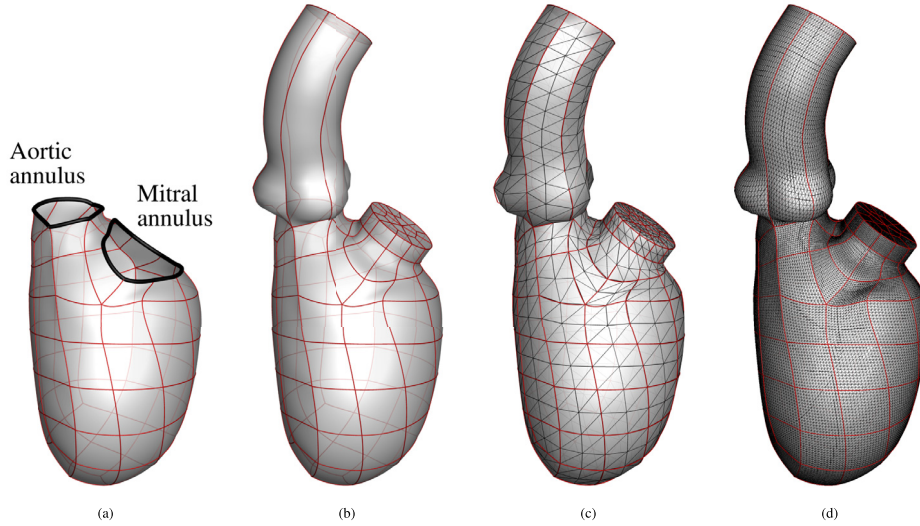


Fig. 1. Reference fluid domain mesh generation: (a) the spline patches making up the left ventricle model; (b) LV model with an idealized aorta and LA extension; (c) coarse triangulation of the model; (d) fine triangulation of the model that is used as the resolution in the FSI simulation.

3.2. Geometry modeling and mesh generation

For this cardiac flow study, the endocardial surface obtained from the cardiac biomechanics simulation is used as an input for the ventricular FSI simulation. Starting from the geometry of the biventricular model described in Section 3.1, we extract the portion that includes the full LV endocardium and the mitral and aortic flow tracts, as shown in Fig. 1(a). We then attach an idealized aorta to the aortic annulus, and a cylindrical LA extension to the mitral annulus to allow flow development before the MV. The smooth annular connections, between the idealized aorta and the aortic annulus, and between the cylindrical LA extension and the mitral annulus, are achieved via cubic spline interpolation. Fig. 1(b) illustrates the geometry that is used for the FSI simulation as the reference configuration, with the edges denoting the patch boundaries. Starting from the reference configuration, the motions of the aorta and the LA extension are prescribed with the following constraints. The centerlines of the aorta and LA extension are only allowed to translate in space from the reference configuration, with their lower endpoints attached to the centers of the aortic and mitral annuli, respectively. The diameters of the aorta and the LA extension are scaled following the change of the aortic and mitral annuli, respectively. Throughout the cardiac cycle, the annular connections are kept smooth.

Due to their flexibility and adaptivity, we use pure tetrahedral elements to discretize the moving fluid domain. We start by discretizing the spline patches into a triangular mesh. Since the spline patches are part of the biventricular finite element mesh, the smoothness between neighboring patches is automatically maintained, and we can split each patch into triangles that share nodes on the patch boundaries (Fig. 1(c)). Note that Fig. 1(c) shows a very coarse mesh that is only used to illustrate the surface discretization. We locate the surface element nodes in the parametric space of the spline patches. The parametric coordinates are used to interpolate the current locations of the nodes when the LV deforms, and are then used as boundary conditions to deform the fluid domain in the FSI simulation. Finally, the volumetric mesh is generated based on the refined surface triangular mesh illustrated in Fig. 1(d). As a result, a total of 1,232,871 elements are generated for the volumetric mesh. The volumetric mesh is updated at each time step by solving the equations of elastostatics [74–76,107], with the prescribed displacement boundary conditions on the surface nodes

extracted from the LV structural motion obtained in Section 3.1 and the aorta and LA motions previously described in this section. Note that the temporal resolution of the LV motion from the structural analysis is limited, so we use periodic cubic splines to smoothly interpolate the LV motion into arbitrarily small time steps.

For the BHVs in this paper, we use the T-spline model from Hsu et al. [51]. The T-spline mesh for the aortic BHV comprises 382 and 1020 Bézier elements for each leaflet and the stent, respectively, and a total of 2262 T-spline control points. The T-spline mesh for the mitral BHV comprises 354 and 1020 Bézier elements for each leaflet and the stent, respectively, and a total of 2169 T-spline control points. We scale and locate the BHVs such that the suture rings of the AV and MV stents match the aortic and mitral annuli, respectively. The sizes of the BHVs for AV and MV replacements are 20 mm and 24 mm (based on stent diameter), respectively. Fig. 2 illustrates the parameterization of the BHV model, and the reference configuration in which two BHVs are implanted into the LV, with the MV replacement placed in an inverted configuration.

The attached edges of the leaflets are clamped to the stent by constraining the relative motions of the two rows of control points adjacent to the stent. These control points are highlighted in Fig. 2. We model the surgical suturing between the BHV stent and the annulus by intersecting the suture ring with the LV wall. Fig. 2 shows the geometric intersection of the stent with the fluid domain boundary. The intersection seals the space between the BHV and the LV fluid domain boundaries, such that the blood can only flow through the orifices of the BHVs when they are open. The intersection is maintained during the entire cardiac cycle by matching the movements of the suture rings to the motions of the AV and MV annuli.

3.3. FSI simulation details

The flow boundary conditions are shown in Fig. 3. In the FSI simulation, we apply the left atrial pressure based on the simulations from Krishnamurthy et al. [70] as a traction boundary condition at the mitral inflow tract. The applied pressure profile, shown in Fig. 3, is periodic with a time period of 0.8 s. A resistance boundary condition is applied at the outflow boundary of the ascending aorta in the form of a traction $-(p_0 + RQ)\mathbf{n}^{\text{out}}$, where p_0 is the end-diastolic aortic pressure, $\mathbf{n}^{\text{out}}$ is the outward-facing normal of the fluid domain, R is a resistance constant, and Q is the volumetric flow rate through the outflow.

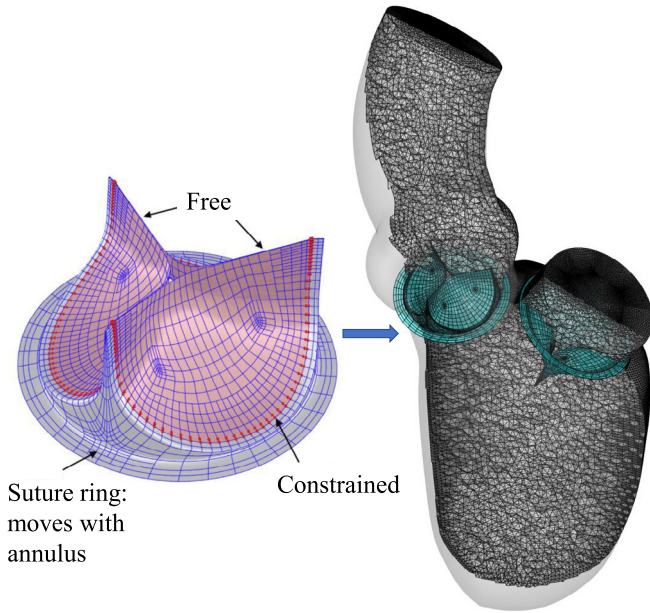


Fig. 2. The BHV model discretization and configuration of the AV and MV implants, which are immersed into the LV fluid domain. The control points with constrained motion are highlighted by red color in the left-hand-side figure. (For interpretation of the references to color in this figure legend, the reader is referred to the web version of this article.)

In the present computation, we set $p_0 = 40$ mmHg and $R = 70$ (dyn s)/cm⁵. The end-diastolic aortic pressure value, which is lower than the normal physiological level, is consistent with the LV structural simulation of a patient who is in the early stages of heart failure with ventricular dyssynchrony that has not progressed to dilated cardiomyopathy [70]. Backflow stabilizations [108] are used at the mitral inflow tract and the aorta outlet boundary, by

adding the following term to the fluid subproblem:

$$-\gamma \sum_i \int_{(\Gamma_i^{\text{out}})_t} \mathbf{w}_i \cdot \{(\mathbf{u}_i - \hat{\mathbf{u}}) \cdot \mathbf{n}_i\}_- \mathbf{u}_i d\Gamma, \quad (12)$$

where $\gamma = 0.5$, $\{(\mathbf{u}_i - \hat{\mathbf{u}}) \cdot \mathbf{n}_i\}_- = \frac{1}{2}((\mathbf{u}_i - \hat{\mathbf{u}}) \cdot \mathbf{n}_i - |(\mathbf{u}_i - \hat{\mathbf{u}}) \cdot \mathbf{n}_i|)$, and $(\Gamma_i^{\text{out}})_t$ is the i th outflow boundary. On all other boundaries, weakly enforced no-slip boundary conditions are applied. The different phases of the cardiac cycle (e.g. the LV systole and diastole) are labeled on the LV volume profile in Fig. 3. The normal and tangential velocity penalization parameters used in our FSI formulation are $\tau_{\text{TAN}}^B = 2.0 \times 10^3$ g/(cm² s) and $\tau_{\text{NOR}}^B = 2.0 \times 10^2$ g/(cm² s). The time step size is $\Delta t = 1.0 \times 10^{-4}$ s so that a total of 8000 time steps are used in a complete cardiac cycle. The fluid density and viscosity in the fluid domain are set as $\rho_1 = 1.0$ g/cm³ and $\mu = 3.0 \times 10^{-2}$ g/(cm s), respectively, to model the physical properties of human blood [109,110].

Remark 4. The simulations are carried out in a parallel computing environment on the Lonestar5 Linux cluster [111] of the Texas Advanced Computing Center [112]. The system consists of 1252 compute nodes, each with two Intel E5-2690 v3 12-core (Haswell) processors and 64 GB of DDR4 memory. We partition the fluid mesh into 96 subdomains, and use the parallelization strategy presented in Hsu et al. [113]. With these configurations, a complete cardiac cycle takes 38 to 42 h to simulate.

The material parameters in Eq. (10) are set to $c_0 = 5.0 \times 10^6$ dyn/cm², $c_1 = 2.0 \times 10^5$ dyn/cm², and $c_2 = 100.0$. Based on the three-point bending tests of glutaraldehyde-treated bovine pericardium reported by Mirnajafi et al. [114], we set the coefficient c_0 such that it provides a similar small-strain bending stiffness. The parameters c_1 and c_2 are selected based on the assumption that the BHVs in this paper are comparable to the pericardial BHV leaflet models in Sun et al. [115]. The mass density of the leaflets is set to 1.0 g/cm³. The thickness of the leaflets is 0.0386 cm, which is selected as a typical thickness of adult bovine pericardial tissue [116,117]. The stents are assumed to be rigid, considering their large stiffness compared with the leaflets.

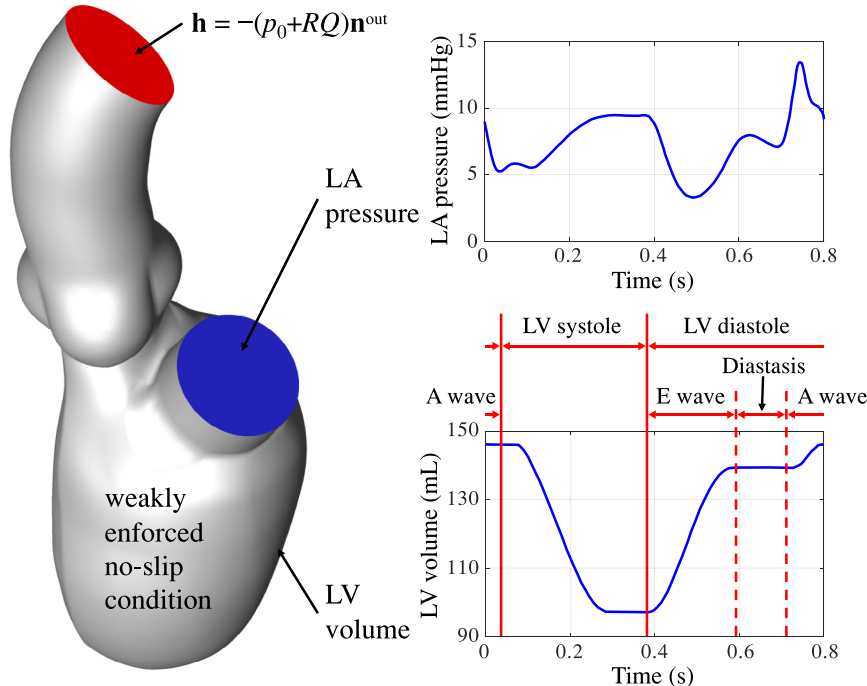


Fig. 3. Setup for the FSI simulation. Different phases of the cardiac cycle are labeled on the LV volume curve.

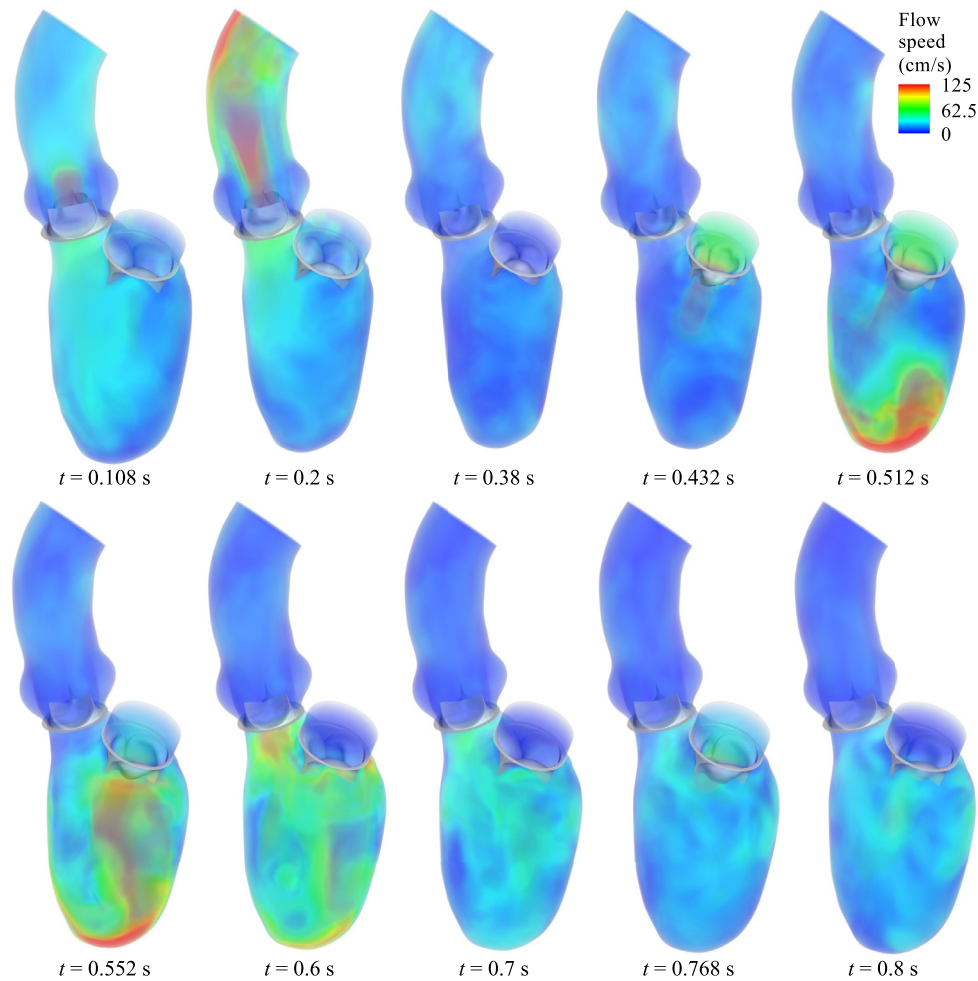


Fig. 4. Visualization of the FSI results for the flow field in the LV and the BHV motions in a complete cardiac cycle.

4. Results and discussions

4.1. FSI simulation results

The FSI simulation is carried out for four cardiac cycles in order to achieve a statistically periodic steady state. To evaluate the variations between cycles, the volumetric flow rate entering the mitral inflow tract is monitored and compared between the third and fourth cycles. The L^2 -norm of flow rate difference between the two cycles is below 3% of the L^2 -norm of fourth-cycle flow rate. All the results presented in this section are based on the fourth cycle. Several snapshots of the BHV deformation and the details of the flow field at several time points during the cardiac cycle are presented in Fig. 4. The visualization of flows and structures clearly demonstrates the response of the valves to the left ventricular motions and hemodynamics. The entire cardiac cycle can be divided into several representative time intervals, as detailed on the LV volume profile in Fig. 3. During the 0.05 s to 0.38 s time interval, the contraction of the LV volume causes the aortic BHV to open and allow blood flow into the aorta. This time period corresponds to the systole of the LV, during which the mitral BHV closes and prevents the flow from reversing to the LA. The next part of the cycle, between 0.38 s and 0.8 s, is the diastole of the LV. In the early diastole (E wave) from 0.38 s to 0.6 s, the mitral BHV fully opens and a large amount of blood fills into the LV chamber while the LV wall relaxes. The mitral BHV closes during the 0.6 s to 0.72 s time period of diastasis. Finally, the atrial contraction during the A wave

propels additional blood flows into the LV, and reopens the mitral BHV at 0.768 s. Due to the shorter duration and lower strength of the A wave, the mitral BHV opening during this period is minor compared to its opening during the E wave. As a result, most of the blood flow transfer from the LA to the LV is completed during the E wave.

Fig. 5 visualizes the vortical structures at the same time frames as Fig. 4. The vortical structures are created using isosurfaces of the second invariant of the velocity gradient matrix, i.e. the λ_2 criterion [118]. Some of the same flow phenomena that were observed in Fig. 4 are also clearly visible from the vortical structures. The vortex ring generated by the mitral jet during LV diastole is one of the most distinguishable features of intraventricular flows. During the E wave, the vortex ring demonstrates that the flow forms a jet as it moves to the apex, from 0.432 s to 0.512 s. Once the blood flow reaches the apex, it reverses and moves upwards toward the valves. The vortical structures at 0.552 s indicate that the flows are well mixed in the LV. During the A wave, the small ring-structured vortex can be clearly observed. This vortex is generated from the minor mitral BHV opening created by the atrial kick from the LA contraction, and moves into the LV while the flows in the other regions remain mostly at rest.

4.2. Effects of BHV on hemodynamic pattern

The asymmetry of the native MV leaflets guides the flow to impinge toward the LV posterior wall [8,9] during LV diastole. The

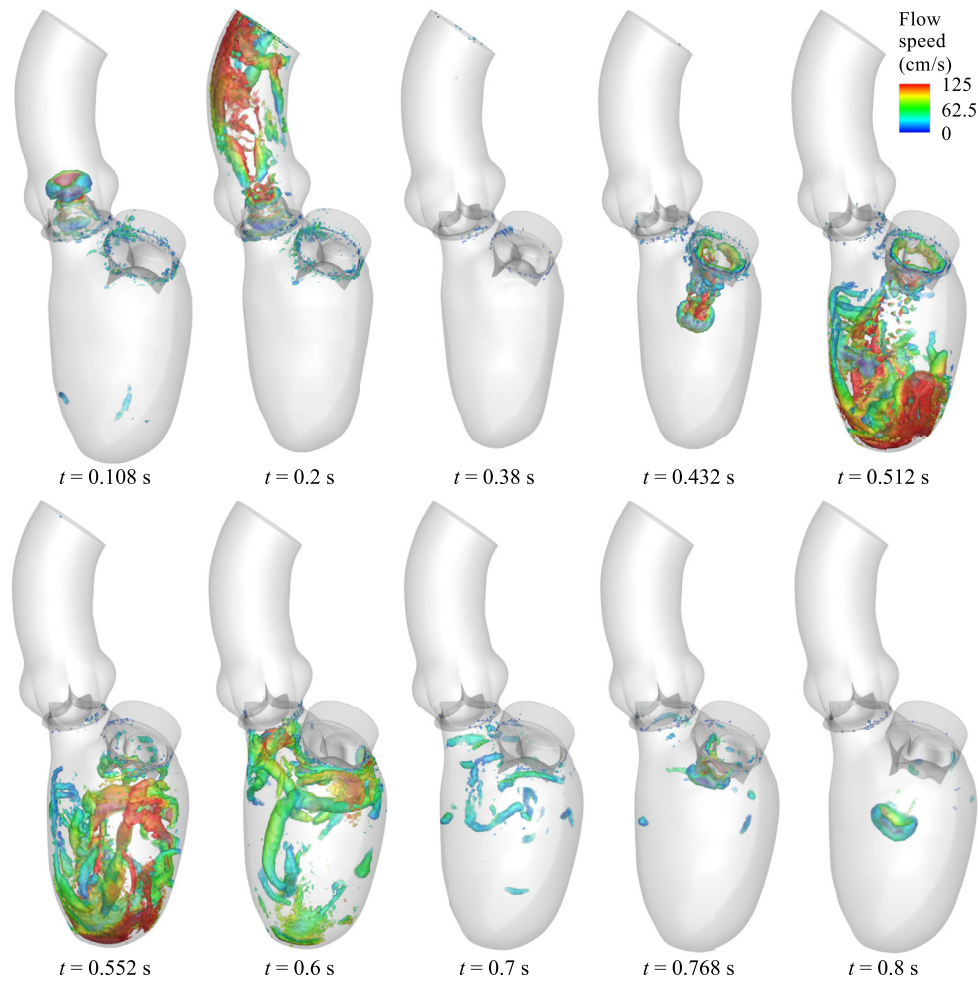


Fig. 5. Vortical structures colored by the velocity magnitude in a complete cardiac cycle.

flow continues in the same direction until it reaches the apex of the LV, where it turns and is redirected toward the outflow tract (the AV annulus). A schematic of the flow pattern is depicted in Fig. 6(a). The jet flow that reaches the apex is considered to be important for enhancing apical washout in the LV [9]. Without proper apical washout, the blood flow could reach a stasis in the apex region and cause subsequent thrombus formation [119,120]. In addition, with the clockwise circulatory pattern, the systolic contraction of the LV would propel blood flow that is already moving toward the aortic valve, such that the momentum loss is minimal.

With the implant of a symmetric BHV in the MV annulus, obvious changes in the flow pattern can be observed. The most prominent change is the direction of the flow jet entering the LV. Fig. 6(b) shows that the flow is essentially perpendicular to the MV annulus plane, and it impacts the interventricular septum instead of impinging toward the posterior wall. Subsequently, the flow turns counterclockwise toward the apex, and the blood flow circulates back toward the MV along the posterior wall, as suggested by Fig. 6(c). As a result, the replacement of the native MV with a symmetric BHV changes the direction of the diastolic vorticity inside the LV. In spite of the direction change of the vorticity, it can be observed that the apical washout is still present. Fig. 6(c) shows a high speed flow, which may result from the smaller orifice areas of BHVs compared to healthy native MVs [6,121], that changes direction in the apex region. From a heart-workload perspective, a negative effect of the high-speed jet is that the resulting large kinetic energy of blood typically indicates increased workload

done by the expanding LV. On the other hand, the high speed jet can actually enhance the apical washout and the blood mixing in the LV, which is desirable as it reduces the risk of stasis [119,120].

Potential adverse effects can also result from the altered pressure distribution in the LV. The impact of the jet on the interventricular septum will increase the pressure on the septum, compared with the native MV case in which the jet moves along the posterior wall, as shown in Fig. 6(d). As a result, the septal tissue may be exposed to higher stresses than those that result from the native MV. In addition, the normal equilibrium developed under pre-implant physiological conditions may be modified after valve replacement. It was also reported that the LV may suffer from changes in geometry after MV replacements [122], which can worsen with the removal of the chordae tendineae during conventional MV replacement surgeries [123,124]. Further studies of these post-operative phenomena, including the effect of hemodynamic changes on LV chamber geometry, are necessary to investigate the subsequent impact of replacing the native MV with a BHV.

5. Conclusions, limitations, and future work

5.1. Conclusions

This study focuses on using advanced hybrid ALE/IMGA modeling and simulation to better understand the hemodynamics in the LV with BHV implants. The structures and kinematics of the BHVs are expected to have a significant influence on the LV hemody-

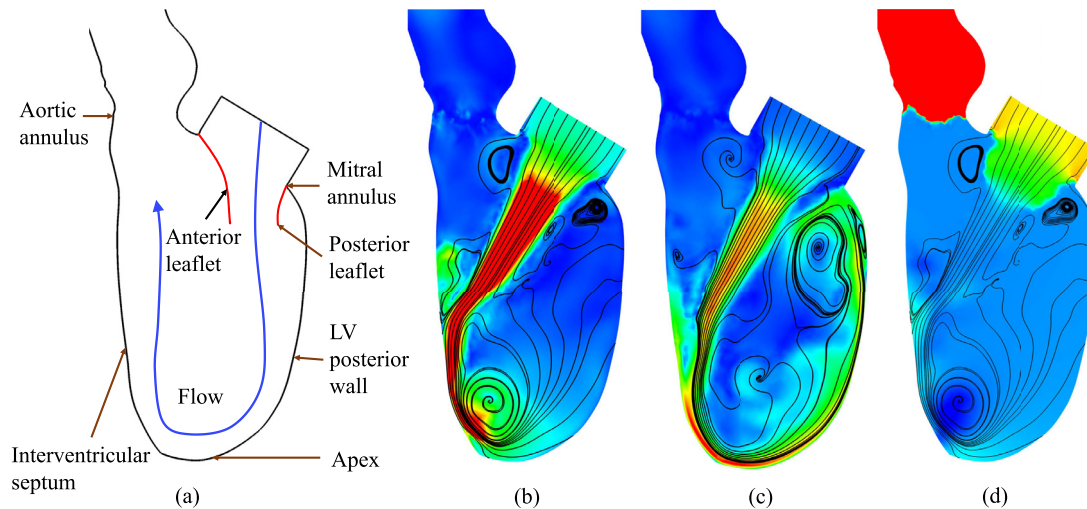


Fig. 6. Comparison of flow circulatory patterns in the LV during diastole: (a) schematic of the flow direction resulting from a typical native valve [8]; (b) streamlines and velocity magnitude contours for the BHV FSI results at $t = 0.472$ s; (c) streamlines and velocity magnitude contours for the BHV FSI results at $t = 0.552$ s; (d) pressure contours at $t = 0.472$ s. Velocity magnitude contours are plotted using a color scale ranging from 0 (blue) to ≥ 200 cm/s (red) in (b) and (c). Pressure contours are plotted using a color scale ranging from ≤ -5 (blue) to ≥ 5 mmHg (red) in (d). (For interpretation of the references to color in this figure legend, the reader is referred to the web version of this article.)

namics. However, the computational challenges presented by such a complex application pose a substantial obstacle for numerical investigations that use classical methods. Such challenges include large-scale structural deformations, as well as contact/impact between heart valve leaflets. To overcome these issues, this work employs the IMGA method to model the interactions between the blood flow and the valve in a non-boundary-fitted approach. Combined with a penalty-based contact algorithm, these methods produce a physiologically realistic valvular FSI modeling approach. In conjunction with these valve models, the ALE-VMS method is utilized to model the hemodynamics that result from LV wall motion, which incorporates the accuracy provided by boundary-fitted approaches. Through the combination of these advanced technologies, numerical simulations of the LV FSI system are carried out using a computational approach that balances robustness and accuracy. These simulation results predict the LV intraventricular flow field after AV and MV replacements. Several unique phenomena in the LV, such as the valve opening and flow behavior that is caused by the atrial kick, are accurately captured. The effect of BHV replacements on the vortex direction reversal in the specific LV presented in this paper is particularly highlighted since this hemodynamic change may have a profound impact on the LV workload and structural behavior.

5.2. Limitations and future work

The primary intent of this paper is to develop an FSI modeling and simulation framework for cardiac and valvular problems. Although this framework is intended to provide a flexible approach to model many cardiac conditions, the presented results and observations are specific to the boundary conditions and geometries specified in this paper, and the conclusions should not be generalized to all other possible variations. In the future, the proposed hybrid ALE/IMGA framework could be applied to simulate a diverse set of cardiac conditions, including variations in boundary conditions and geometries, which would further demonstrate its robustness and physiological realism. The proposed framework could also be extended and applied to different cardiac applications, especially those hearts with prosthetic valve replacements, and to include four-chamber models [104] and atrioventricular valves [125,126]. Efficiently exploring the myriad of parameters

that are present in the wide variety of cardiac problems would require some form of automated optimization. Previous work has demonstrated that the FSI system can be optimized using a surrogate management framework (SMF) [127], and similar combinations of the SMF and hybrid ALE/IMGA framework could provide an effective tool for future numerical studies of cardiac systems.

The specific heart geometry in this paper is from a patient with mild heart failure with ventricular dyssynchrony that has not progressed to dilated cardiomyopathy [70]. The cardiac motion for such a patient in the early stages of heart failure is expected to remain within a normal range. Although the LV motion and the boundary conditions in this paper are within a reasonable range, the following assumptions and simplifications had to be taken to make the FSI simulation more tractable. First, all the motions of the boundaries, including the LV and the ascending aorta, are prescribed. With the BHV replacements, the altered pressure may not be consistent with the prescribed volume change, and as a result, the effect of LV and aorta compliance is likely not well reproduced. In addition, the LA is simplified to a cylindrical section that is attached to the mitral inflow tract, which artificially alters the mechanism driving the flow through the MV during the A wave. Instead of being driven by the contraction of LA, the flow is driven by the suction created by the prescribed LV volume expansion. This explains the LV pressure profile discrepancy in Fig. 7 between 0.72 s and 0.8 s, where an obvious pressure drop is observed in the FSI simulated LV pressure. Some other limitations of this work include the simple resistance boundary condition applied at the outlet of the ascending aorta. This limitation can be addressed in the future by incorporating Windkessel-type boundary conditions [128].

The paradigm proposed in this work provides an effective tool to better understand the fluid and structural behaviors in the cardiac system. Despite the realistic modeling approaches presented in this work, the BHV structures and the deformation of the LV are limited to the idealized data that is available for these geometries and the structural simulation of the LV. The simplification of these model inputs produces more idealized FSI simulation results that will be improved in the future by connecting the present hybrid ALE/IMGA framework to medical imaging technologies [52]. Incorporating these data has significant potential to lead to highly realistic patient-specific modeling and simulation. Such an integrated tool could be beneficial for developing novel implant strategies

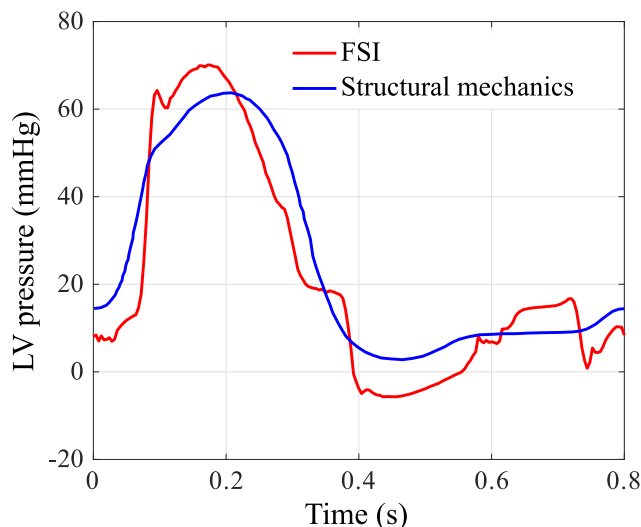


Fig. 7. The intraventricular pressure of the FSI simulation throughout a complete cardiac cycle. The intraventricular pressure is obtained by space-averaging the blood pressure in the LV. The LV pressure used in the structural mechanics simulation of the LV motion is plotted for reference.

that focus on replicating the native blood flows after BHV replacement operations. Eventually, this physics-based computational FSI framework could help reduce the morbidity and mortality in cardiac disease treatments through improved surgical planning and personalized medical device design.

Declaration of Competing Interest

The authors declare no conflict of interest.

Acknowledgments

E.L. Johnson, M.S. Sacks, and M.-C. Hsu were partially supported by the National Heart, Lung, and Blood Institute of the National Institutes of Health under award numbers R01HL129077 and R01HL142504. A. Krishnamurthy was partially supported by the same institute under award number R01HL131753 and by the National Science Foundation under award number 1750865. All this support is gratefully acknowledged. We also thank the Texas Advanced Computing Center (TACC) at The University of Texas at Austin for providing HPC resources that have contributed to the research results reported in this paper.

References

- [1] A.P. Yoganathan, Z. He, S.C. Jones, Fluid mechanics of heart valves, *Annu. Rev. Biomed. Eng.* 6 (2004) 331–362.
- [2] R.A. Nishimura, C.M. Otto, R.O. Bonow, B.A. Carabello, J.P. Erwin, R.A. Guyton, P.T. O’Gara, C.E. Ruiz, N.J. Skubas, P. Sorajja, T.M. Sundt, J.D. Thomas, 2014 AHA/ACC Guideline for the management of patients with valvular heart disease, *Circulation* 129 (2014) e521–e643.
- [3] R.L. Li, J. Russ, C. Paschalides, G. Ferrari, H. Waisman, J.W. Kysar, D. Kalfa, Mechanical considerations for polymeric heart valve development: biomechanics, materials, design and manufacturing, *Biomaterials* 225 (2019) 119493.
- [4] F.J. Schoen, J. Butany, Cardiac valve replacement and related interventions, in: *Cardiovascular Pathology*, Elsevier, 2016, pp. 529–576.
- [5] J.S. Soares, K.R. Feaver, W. Zhang, D. Kamensky, A. Aggarwal, M.S. Sacks, Biomechanical behavior of bioprosthetic heart valve heterograft tissues: characterization, simulation, and performance, *Cardiovasc. Eng. Technol.* 7 (4) (2016) 309–351.
- [6] J. Magne, P. Mathieu, J.G. Dumesnil, D. Tanné, F. Dagenais, D. Doyle, P. Pibarot, Impact of prosthesis-patient mismatch on survival after mitral valve replacement, *Circulation* 115 (2007) 1417–1425.
- [7] W.B. Eichinger, F. Botzenhardt, R. Gunzinger, B.M. Kemkes, A. Sosnowski, D. Maiza, E.O. Coto, N. Bleese, European experience with the mosaic bioprosthesis, *J. Thorac. Cardiovasc. Surg.* 124 (2) (2002) 333–339.

- [8] G. Pedrizzetti, F. Domenichini, G. Tonti, On the left ventricular vortex reversal after mitral valve replacement, *Ann. Biomed. Eng.* 38 (3) (2010) 769–773.
- [9] J.H. Seo, V. Vedula, T. Abraham, A.C. Lardo, F. Dawoud, H. Luo, R. Mittal, Effect of the mitral valve on diastolic flow patterns, *Phys. Fluids* 26 (12) (2014) 121901.
- [10] S.H. Daebritz, J.S. Sachweh, B. Hermanns, B. Fausten, A. Franke, J. Groetzner, B. Klosterhalfen, B.J. Messmer, Introduction of a flexible polymeric heart valve prosthesis with special design for mitral position, *Circulation* 108 (2003) II–134–II–139.
- [11] H. Mächler, M. Perthel, G. Reiter, U. Reiter, M. Zink, P. Bergmann, A. Waltensdorfer, J. Laas, Influence of bileaflet prosthetic mitral valve orientation on left ventricular flow—an experimental in vivo magnetic resonance imaging study, *Eur. J. Cardio-Thoracic Surgery* 26 (4) (2004) 747–753.
- [12] J. Turina, T. Stark, B. Seifert, M. Turina, Predictors of the long-term outcome after combined aortic and mitral valve surgery, *Circulation* 100 (suppl II) (1999) II–48–II–53.
- [13] C.J. Carmody, G. Burriesci, I.C. Howard, E.A. Patterson, An approach to the simulation of fluid–structure interaction in the aortic valve, *J. Biomech.* 39 (1) (2006) 158–169.
- [14] S.K. Dahl, J. Vierendeels, J. Degroote, S. Annerel, L.R. Hellevik, B. Skallerud, FSI Simulation of asymmetric mitral valve dynamics during diastolic filling, *Comput. Methods Biomech. Biomed. Eng.* 15 (2) (2012) 121–130.
- [15] T.B. Le, F. Sotiropoulos, On the three-dimensional vortical structure of early diastolic flow in a patient-specific left ventricle, *Eur. J. Mech. B/Fluids* 35 (2012) 20–24.
- [16] T.B. Le, F. Sotiropoulos, Fluid–structure interaction of an aortic heart valve prosthesis driven by an animated anatomic left ventricle, *J. Comput. Phys.* 244 (2013) 41–62.
- [17] A.L. Marsden, I.E. Vignon-Clementel, F. Chan, J.A. Feinstein, C.A. Taylor, Effects of exercise and respiration on hemodynamic efficiency in CFD simulations of the total cavopulmonary connection, *Ann. Biomed. Eng.* 35 (2007) 250–263.
- [18] A.L. Marsden, A.D. Bernstein, V.M. Reddy, S. Shadden, R. Spilker, F.P. Chan, C.A. Taylor, J.A. Feinstein, Evaluation of a novel y-shaped extracardiac fontan baffle using computational fluid dynamics, *J. Thorac. Cardiovasc. Surgery* 137 (2009) 394–403.e2.
- [19] H.J. Kim, I.E. Vignon-Clementel, J.S. Coogan, C.A. Figueroa, K.E. Jansen, C.A. Taylor, Patient-specific modeling of blood flow and pressure in human coronary arteries, *Ann. Biomed. Eng.* 38 (10) (2010) 3195–3209.
- [20] A.S. Les, S.C. Shadden, C.A. Figueroa, J.M. Park, M.M. Tedesco, R.J. Herfkens, R.L. Dalman, C.A. Taylor, Quantification of hemodynamics in abdominal aortic aneurysms during rest and exercise using magnetic resonance imaging and computational fluid dynamics, *Ann. Biomed. Eng.* 38 (4) (2010) 1288–1313.
- [21] P. Eslami, J. Tran, Z. Jin, J. Karady, R. Sotodeh, M.T. Lu, U. Hoffmann, A. Marsden, Effect of wall elasticity on hemodynamics and wall shear stress in patient-specific simulations in the coronary arteries, *J. Biomech. Eng.* 142 (2) (2020) 024503.
- [22] C.A. Taylor, T.A. Fonte, J.K. Min, Computational fluid dynamics applied to cardiac computed tomography for noninvasive quantification of fractional flow reserve: scientific basis, *J. Am. Coll. Cardiol.* 61 (22) (2013) 2233–2241.
- [23] J.M. Lee, G. Choi, D. Hwang, J. Park, H.J. Kim, J.-H. Doh, C.-K. Nam, S.-H. Na, E.-S. Shin, C.A. Taylor, B.-K. Koo, Impact of longitudinal lesion geometry on location of plaque rupture and clinical presentations, *JACC: Cardiovasc. Imaging* 10 (6) (2017) 677–688.
- [24] C.A. Taylor, S. Gaur, J. Leipsic, S. Achenbach, D.S. Berman, J.M. Jensen, D. Dey, H.E. Botker, H.J. Kim, S. Khem, A. Wilk, C.K. Zarins, H. Bezerra, J. Lesser, B. Ko, J. Narula, A. Ahmadi, K.A. Øvrehus, F. St Goar, B. De Bruyne, B.L. Nørgaard, Effect of the ratio of coronary arterial lumen volume to left ventricle myocardial mass derived from coronary CT angiography on fractional flow reserve, *J. Cardiovasc. Comput. Tomogr.* 11 (6) (2017) 429–436.
- [25] B.N. Modi, S. Sankaran, H.J. Kim, H. Ellis, C. Rogers, C.A. Taylor, R. Rajani, D. Perera, Predicting the physiological effect of revascularization in serially diseased coronary arteries: clinical validation of a novel CT coronary angiography-based technique, *Circulat. Cardiovasc. Intervent.* 12 (2) (2019) e007577.
- [26] S.N. Doost, L. Zhong, B. Su, Y.S. Morsi, The numerical analysis of non-Newtonian blood flow in human patient-specific left ventricle, *Comput. Methods Progr. Biomed.* 127 (2016) 232–247.
- [27] A.M. Bavo, A.M. Pouch, J. Degroote, J. Vierendeels, J.H. Gorman, R.C. Gorman, P. Segers, Patient-specific CFD simulation of intraventricular haemodynamics based on 3D ultrasound imaging, *Biomed. Eng. Online* 15 (1) (2016) 107.
- [28] A.M. Bavo, A.M. Pouch, J. Degroote, J. Vierendeels, J.H. Gorman, R.C. Gorman, P. Segers, Patient-specific CFD models for intraventricular flow analysis from 3D ultrasound imaging: comparison of three clinical cases, *J. Biomech.* 50 (2017) 144–150.
- [29] W. Mao, A. Caballero, R. McKay, C. Primiano, W. Sun, Fully-coupled fluid–structure interaction simulation of the aortic and mitral valves in a realistic 3D left ventricle model, *PLoS ONE* 12 (9) (2017) e0184729.
- [30] T. Terahara, K. Takizawa, T.E. Tezduyar, A. Tsushima, S. K., Ventricle-valve-aorta flow analysis with the space-time isogeometric discretization and topology change, *Comput. Mech.* 65 (2020) 1343–1363.
- [31] R. Mittal, J.H. Seo, V. Vedula, V.J. Choi, H. Liu, H.H. Huang, S. Jain, L. Younes, T. Abraham, R.T. George, Computational modeling of cardiac hemodynamics: current status and future outlook, *J. Comput. Phys.* 305 (2016) 1065–1082.
- [32] T.J.R. Hughes, W.K. Liu, T.K. Zimmermann, Lagrangian–eulerian finite element formulation for incompressible viscous flows, *Comput. Methods Appl. Mech. Eng.* 29 (1981) 329–349.

- [33] J. Donea, S. Giuliani, J.P. Halleux, An arbitrary Lagrangian–Eulerian finite element method for transient dynamic fluid–structure interactions, *Comput. Methods Appl. Mech. Eng.* 33 (1–3) (1982) 689–723.
- [34] J. Donea, A. Huerta, J.-P. Ponthot, A. Rodríguez-Ferran, Arbitrary Lagrangian–Eulerian methods, in: *Encyclopedia of Computational Mechanics*, John Wiley & Sons, 2004.
- [35] T.E. Tezduyar, M. Behr, J. Liou, A new strategy for finite element computations involving moving boundaries and interfaces – the deforming-spatial-domain/space-time procedure: I. the concept and the preliminary numerical tests, *Comput. Methods Appl. Mech. Eng.* 94 (3) (1992a) 339–351.
- [36] T.E. Tezduyar, M. Behr, S. Mittal, J. Liou, A new strategy for finite element computations involving moving boundaries and interfaces – the deforming-spatial-domain/space-time procedure: II. computation of free-surface flows, two-liquid flows, and flows with drifting cylinders, *Comput. Methods Appl. Mech. Eng.* 94 (3) (1992b) 353–371.
- [37] T.E. Tezduyar, K. Takizawa, Space-time computations in practical engineering applications: a summary of the 25-year history, *Comput. Mech.* 63 (2019) 747–753.
- [38] K. Takizawa, T.E. Tezduyar, T. Sasaki, Aorta modeling with the element-based zero-stress state and isogeometric discretization, *Comput. Mech.* 59 (2017) 265–280.
- [39] T. Sasaki, K. Takizawa, T.E. Tezduyar, Aorta zero-stress state modeling with T-spline discretization, *Comput. Mech.* 63 (2019) 1315–1331.
- [40] K. Takizawa, T.E. Tezduyar, H. Uchikawa, T. Terahara, T. Sasaki, A. Yoshida, Mesh refinement influence and cardiac-cycle flow periodicity in aorta flow analysis with isogeometric discretization, *Comput. Fluids* 179 (2019) 790–798.
- [41] T. Sasaki, K. Takizawa, T.E. Tezduyar, Medical-image-based aorta modeling with zero-stress-state estimation, *Comput. Mech.* 64 (2019) 249–271.
- [42] Y. Yu, Y.J. Zhang, K. Takizawa, T.E. Tezduyar, T. Sasaki, Anatomically realistic lumen motion representation in patient-specific space-time isogeometric flow analysis of coronary arteries with time-dependent medical-image data, *Comput. Mech.* 65 (2) (2020) 395–404.
- [43] A.A. Johnson, T.E. Tezduyar, Parallel computation of incompressible flows with complex geometries, *Int. J. Numer. Methods Fluids* 24 (1997a) 1321–1340.
- [44] A.A. Johnson, T.E. Tezduyar, 3D simulation of fluid-particle interactions with the number of particles reaching 100, *Comput. Methods Appl. Mech. Eng.* 145 (1997b) 301–321.
- [45] A.A. Johnson, T.E. Tezduyar, Advanced mesh generation and update methods for 3D flow simulations, *Comput. Mech.* 23 (1999) 130–143.
- [46] S. Sathe, T.E. Tezduyar, Modeling of fluid–structure interactions with the space-time finite elements: contact problems, *Comput. Mech.* 43 (2008) 51–60.
- [47] K. Takizawa, T.E. Tezduyar, T. Terahara, T. Sasaki, Heart valve flow computation with the integrated space-time VMS, slip interface, topology change and isogeometric discretization methods, *Comput. Fluids* 158 (2017) 176–188.
- [48] T. Terahara, K. Takizawa, T.E. Tezduyar, Y. Bazilevs, M.-C. Hsu, Heart valve isogeometric sequentially-coupled FSI analysis with the space-time topology change method, *Comput. Mech.* 65 (2020) 1167–1187.
- [49] D. Kamensky, M.-C. Hsu, D. Schilling, J.A. Evans, A. Aggarwal, Y. Bazilevs, M.S. Sacks, T.J.R. Hughes, An immersogeometric variational framework for fluid–structure interaction: application to bioprosthetic heart valves, *Comput. Methods Appl. Mech. Eng.* 284 (2015) 1005–1053.
- [50] M.-C. Hsu, D. Kamensky, Y. Bazilevs, M.S. Sacks, T.J.R. Hughes, Fluid–structure interaction analysis of bioprosthetic heart valves: significance of arterial wall deformation, *Comput. Mech.* 54 (2014) 1055–1071.
- [51] M.-C. Hsu, D. Kamensky, F. Xu, J. Kiendl, C. Wang, M.C.H. Wu, J. Mineroff, A. Reali, Y. Bazilevs, M.S. Sacks, Dynamic and fluid–structure interaction simulations of bioprosthetic heart valves using parametric design with T-splines and Fung-type material models, *Comput. Mech.* 55 (2015) 1211–1225.
- [52] F. Xu, S. Morganti, R. Zakerzadeh, D. Kamensky, F. Auricchio, A. Reali, T.J.R. Hughes, M.S. Sacks, M.-C. Hsu, A framework for designing patient-specific bioprosthetic heart valves using immersogeometric fluid–structure interaction analysis, *Int. J. Numer. Methods Biomed. Eng.* 34 (4) (2018) e2938.
- [53] M.C.H. Wu, R. Zakerzadeh, D. Kamensky, J. Kiendl, M.S. Sacks, M.-C. Hsu, An anisotropic constitutive model for immersogeometric fluid–structure interaction analysis of bioprosthetic heart valves, *J. Biomech.* 74 (2018) 23–31.
- [54] E.L. Johnson, M.C.H. Wu, F. Xu, N.M. Wiese, M.R. Rajanna, A.J. Herrema, B. Ganapathysubramanian, T.J.R. Hughes, M.S. Sacks, M.-C. Hsu, Thinner biological tissues induce leaflet flutter in aortic heart valve replacements, *Proceedings of the National Academy of Sciences* 117 (2020) 19007–19016.
- [55] F. Xu, D. Schilling, D. Kamensky, V. Varduhn, C. Wang, M.-C. Hsu, The tetrahedral finite cell method for fluids: immersogeometric analysis of turbulent flow around complex geometries, *Computers & Fluids* 141 (2016) 135–154.
- [56] M.-C. Hsu, C. Wang, F. Xu, A.J. Herrema, A. Krishnamurthy, Direct immersogeometric fluid flow analysis using B-rep CAD models, *Comput. Aided Geom. Des.* 43 (2016) 143–158.
- [57] C. Wang, F. Xu, M.-C. Hsu, A. Krishnamurthy, Rapid B-rep model preprocessing for immersogeometric analysis using analytic surfaces, *Comput. Aided Geom. Des.* 52–53 (2017) 190–204.
- [58] F. Xu, Y. Bazilevs, M.-C. Hsu, Immersogeometric analysis of compressible flows with application to aerodynamic simulation of rotorcraft, *Math. Models Methods Appl. Sci.* 29 (2019) 905–938.
- [59] Q. Zhu, F. Xu, S. Xu, M.-C. Hsu, J. Yan, An immersogeometric formulation for free-surface flows with application to marine engineering problems, *Comput. Methods Appl. Mech. Eng.* 361 (2020) 112748.
- [60] S. Xu, F. Xu, A. Kommajosula, M.-C. Hsu, B. Ganapathysubramanian, Immersogeometric analysis of moving objects in incompressible flows, *Comput. Fluids* 189 (2019) 24–33.
- [61] M.C.H. Wu, H.M. Muchowski, E.L. Johnson, M.R. Rajanna, M.-C. Hsu, Immersogeometric fluid–structure interaction modeling and simulation of transcatheter aortic valve replacement, *Comput. Methods Appl. Mech. Eng.* 357 (2019) 112556.
- [62] P. Wriggers, *Computational Contact Mechanics*, 2nd ed., Springer-Verlag, Berlin Heidelberg, 2006.
- [63] T.A. Laursen, *Computational Contact and Impact Mechanics: Fundamentals of Modeling Interfacial Phenomena in Nonlinear Finite Element Analysis*, Springer-Verlag, Berlin Heidelberg, 2003.
- [64] D. Kamensky, J.A. Evans, M.-C. Hsu, Stability and conservation properties of collocated constraints in immersogeometric fluid–thin structure interaction analysis, *Commun. Comput. Phys.* 18 (2015) 1147–1180.
- [65] Y. Yu, D. Kamensky, M.-C. Hsu, X.Y. Lu, Y. Bazilevs, T.J.R. Hughes, Error estimates for projection-based dynamic augmented Lagrangian boundary condition enforcement, with application to fluid–structure interaction, *Math. Models Methods Appl. Sci.* 28 (12) (2018) 2457–2509.
- [66] M.-C. Hsu, D. Kamensky, Immersogeometric analysis of bioprosthetic heart valves, using the dynamic augmented Lagrangian method, in: T.E. Tezduyar (Ed.), *Frontiers in Computational Fluid–Structure Interaction and Flow Simulation*, Springer International Publishing, Cham, 2018, pp. 167–212.
- [67] M.-C. Hsu, C. Wang, A.J. Herrema, D. Schilling, A. Ghoshal, Y. Bazilevs, An interactive geometry modeling and parametric design platform for isogeometric analysis, *Comput. Math. Appl.* 70 (2015) 1481–1500.
- [68] Y. Bazilevs, V.M. Calo, J.A. Cottrell, T.J.R. Hughes, A. Reali, G. Scovazzi, Variational multiscale residual-based turbulence modeling for large eddy simulation of incompressible flows, *Comput. Methods Appl. Mech. Eng.* 197 (2007) 173–201.
- [69] J. Kiendl, M.-C. Hsu, M.C.H. Wu, A. Reali, Isogeometric Kirchhoff–Love shell formulations for general hyperelastic materials, *Comput. Methods Appl. Mech. Eng.* 291 (2015) 280–303.
- [70] A. Krishnamurthy, C.T. Villongco, J. Chuang, L.R. Frank, V. Nigam, E. Belezouli, P. Stark, D.E. Krummen, S. Narayan, J.H. Omens, A.D. McCulloch, R.C.P. Kerckhoffs, Patient-specific models of cardiac biomechanics, *J. Comput. Phys.* 244 (2013) 4–21.
- [71] D. Kamensky, F. Xu, C.-H. Lee, J. Yan, Y. Bazilevs, M.-C. Hsu, A contact formulation based on a volumetric potential: application to isogeometric simulations of atrioventricular valves, *Comput. Methods Appl. Mech. Eng.* 330 (2018) 522–546.
- [72] A. Krishnamurthy, M.J. Gonzales, G. Sturgeon, W.P. Segars, A.D. McCulloch, Biomechanics simulations using cubic Hermite meshes with extraordinary nodes for isogeometric cardiac modeling, *Comput. Aided Geom. Des.* 43 (2016) 27–38.
- [73] Y. Bazilevs, M.-C. Hsu, M.A. Scott, Isogeometric fluid–structure interaction analysis with emphasis on non-matching discretizations, and with application to wind turbines, *Comput. Methods Appl. Mech. Eng.* 249 (2012) 28–41.
- [74] T.E. Tezduyar, Finite element methods for flow problems with moving boundaries and interfaces, *Arch. Comput. Methods Eng.* 8 (2001) 83–130.
- [75] K. Stein, T. Tezduyar, R. Benney, Mesh moving techniques for fluid–structure interactions with large displacements, *J. Appl. Mech.* 70 (2003) 58–63.
- [76] T.E. Tezduyar, S. Sathe, Modeling of fluid–structure interactions with the space-time finite elements: solution techniques, *Int. J. Numer. Methods Fluids* 54 (2007) 855–900.
- [77] J.-F. Gerbeau, M. Vidrascu, P. Frey, Fluid–structure interaction in blood flows on geometries based on medical imaging, *Comput. Struct.* 83 (2005) 155–165.
- [78] F. Nobile, C. Vergara, An effective fluid–structure interaction formulation for vascular dynamics by generalized robin conditions, *SIAM J. Scient. Comput.* 30 (2008) 731–763.
- [79] K. Takizawa, Y. Bazilevs, T.E. Tezduyar, C.C. Long, A.L. Marsden, K. Schjodt, ST and ALE-VMS methods for patient-specific cardiovascular fluid mechanics modeling, *Math. Models Methods Appl. Sci.* 24 (12) (2014) 2437–2486.
- [80] A. Masud, R.A. Khurram, A multiscale finite element method for the incompressible Navier–Stokes equations, *Comput. Methods Appl. Mech. Eng.* 195 (2006) 1750–1777.
- [81] R.A. Khurram, A. Masud, A multiscale/stabilized formulation of the incompressible Navier–Stokes equations for moving boundary flows and fluid–structure interaction, *Comput. Mech.* 38 (2006) 403–416.
- [82] R. Calderer, A. Masud, A multiscale stabilized ALE formulation for incompressible flows with moving boundaries, *Comput. Mech.* 46 (2010) 185–197.
- [83] A. Masud, R. Calderer, Residual-based turbulence models for moving boundary flows: hierarchical application of variational multiscale method and three-level scale separation, *Int. J. Numer. Methods Fluids* 73 (3) (2013) 284–305.
- [84] R. Calderer, L. Zhu, R. Gibson, A. Masud, Residual-based turbulence models and arbitrary lagrangian–Eulerian framework for free surface flows, *Math. Models Methods Appl. Sci.* 25 (12) (2015) 2287–2317.
- [85] A.N. Brooks, T.J.R. Hughes, Streamline upwind/Petrov–Galerkin formulations for convection dominated flows with particular emphasis on the incompressible Navier–Stokes equations, *Comput. Methods Appl. Mech. Eng.* 32 (1982) 199–259.
- [86] T.J.R. Hughes, L. Mazzei, A.A. Oberai, A. Wray, The multiscale formulation of large eddy simulation: decay of homogeneous isotropic turbulence, *Physics of Fluids* 13 (2001) 505–512.

- [87] Y. Bazilevs, J. Yan, M. de Stadler, S. Sarkar, Computation of the flow over a sphere at $Re = 3700$: a comparison of uniform and turbulent inflow conditions, *J. Appl. Mech.* 81 (12) (2014) 121003.
- [88] J. Yan, X. Deng, A. Korobenko, Y. Bazilevs, Free-surface flow modeling and simulation of horizontal-axis tidal-stream turbines, *Comput. Fluids* 158 (2017a) 157–166.
- [89] J. Yan, A. Korobenko, A. Tejada-Martínez, R. Golshan, Y. Bazilevs, A new variational multiscale formulation for stratified incompressible turbulent flows, *Comput. Fluids* 158 (2017b) 150–156.
- [90] Y. Bazilevs, T.J.R. Hughes, Weak imposition of Dirichlet boundary conditions in fluid mechanics, *Comput. Fluids* 36 (2007) 12–26.
- [91] J. Yan, B. Augier, A. Korobenko, J. Czarnowski, G. Ketterman, Y. Bazilevs, FSI modeling of a propulsion system based on compliant hydrofoils in a tandem configuration, *Comput. Fluids* 141 (2016) 201–211.
- [92] Q. Zhu, J. Yan, A moving-domain CFD solver in FEniCS with applications to tidal turbine simulations in turbulent flows, *Comput. Math. Appl.* (2019). <https://doi.org/10.1016/j.camwa.2019.07.034>
- [93] P. Tong, Y.-C. Fung, The stress-strain relationship for the skin, *J. Biomech.* 9 (10) (1976) 649–657.
- [94] Y.-C. Fung, *Biomechanics: Mechanical Properties of Living Tissues*, 2nd ed., Springer-Verlag, New York, 1993.
- [95] W. Sun, M.S. Sacks, T.L. Sellaro, W.S. Slaughter, M.J. Scott, Biaxial mechanical response of bioprosthetic heart valve biomaterials to high in-plane shear, *J. Biomech. Eng.* 125 (3) (2003) 372–380.
- [96] R. Fan, M.S. Sacks, Simulation of planar soft tissues using a structural constitutive model: finite element implementation and validation, *J. Biomech.* 47 (9) (2014) 2043–2054.
- [97] D. Kamensky, M. Behzadinasab, J.T. Foster, Y. Bazilevs, Peridynamic modeling of frictional contact, *J. Peridyn. Nonlocal Model.* 1 (2) (2019) 107–121.
- [98] J. Chung, G.M. Hulbert, A time integration algorithm for structural dynamics with improved numerical dissipation: the generalized- α method, *J. Appl. Mech.* 60 (1993) 371–375.
- [99] J.C. Simo, P. Wriggers, R.L. Taylor, A perturbed lagrangian formulation for the finite element solution of contact problems, *Comput. Methods Appl. Mech. Eng.* 50 (2) (1985) 163–180.
- [100] D. Kamensky, M.-C. Hsu, Y. Yu, J.A. Evans, M.S. Sacks, T.J.R. Hughes, Immersogeometric cardiovascular fluid–structure interaction analysis with divergence-conforming B-splines, *Comput. Methods Appl. Mech. Eng.* 314 (2017) 408–472.
- [101] T.E. Tezduyar, K. Takizawa, C. Moorman, S. Wright, J. Christopher, Space–time finite element computation of complex fluid–structure interactions, *Int. J. Numer. Methods Fluids* 64 (2010) 1201–1218.
- [102] L.E. Hudsmith, S.E. Petersen, J.M. Francis, M.D. Robson, S. Neubauer, Normal human left and right ventricular and left atrial dimensions using steady state free precession magnetic resonance imaging, *J. Cardiovasc. Magnet. Reson.* 7 (5) (2005) 775–782.
- [103] M.J. Gonzales, G. Sturgeon, A. Krishnamurthy, J. Hake, R. Jonas, P. Stark, W.-J. Rappel, S.M. Narayan, Y. Zhang, W.P. Segars, A.D. McCulloch, A three-dimensional finite element model of human atrial anatomy: new methods for cubic hermite meshes with extraordinary vertices, *Med. Image Anal.* 17 (5) (2013) 525–537.
- [104] A. Jafari, E. Pszczolkowski, A. Krishnamurthy, A framework for biomechanics simulations using four-chamber cardiac models, *J. Biomech.* 91 (2019) 92–101.
- [105] G.A. Holzapfel, R.W. Ogden, Constitutive modelling of passive myocardium: a structurally based framework for material characterization, *Philosoph. Trans. R. Soc. A* 367 (1902) (2009) 3445–3475.
- [106] J. Lumens, T. Delhaas, B. Kim, T. Arts, Three-wall segment (triseq) model describing mechanics and hemodynamics of ventricular interaction, *Ann. Biomed. Eng.* 37 (11) (2009) 2234–2255.
- [107] T.E. Tezduyar, M. Behr, S. Mittal, A.A. Johnson, Computation of unsteady incompressible flows with the finite element methods – Space–time formulations, iterative strategies and massively parallel implementations, in: *New Methods in Transient Analysis*, in: PVP-Vol.246/AMD-Vol.143, ASME, New York, 1992, pp. 7–24.
- [108] M. Esmaily-Moghadam, Y. Bazilevs, T.-Y. Hsia, I.E. Vignon-Clementel, A.L. Marsden, A comparison of outlet boundary treatments for prevention of backflow divergence with relevance to blood flow simulations, *Comput. Mech.* 48 (2011) 277–291.
- [109] T. Kenner, The measurement of blood density and its meaning, *Basic Res. Cardiol.* 84 (2) (1989) 111–124.
- [110] R. Rosencranz, S.A. Bogen, Clinical laboratory measurement of serum, plasma, and blood viscosity, *Am. J. Clin. Pathol.* 125 (2006) 78–86.
- [111] TACC Lonestar5 User Guide. <https://portal.tacc.utexas.edu/user-guides/lonestar5>, 2020.
- [112] Texas Advanced Computing Center (TACC), <http://www.tacc.utexas.edu>, 2020.
- [113] M.-C. Hsu, I. Akkerman, Y. Bazilevs, High-performance computing of wind turbine aerodynamics using isogeometric analysis, *Comput. Fluids* 49 (2011) 93–100.
- [114] A. Mirnajafi, J. Raymer, M.J. Scott, M.S. Sacks, The effects of collagen fiber orientation on the flexural properties of pericardial heterograft biomaterials, *Biomaterials* 26 (7) (2005) 795–804.
- [115] W. Sun, A. Abad, M.S. Sacks, Simulated bioprosthetic heart valve deformation under quasi-static loading, *J. Biomech. Eng.* 127 (6) (2005) 905–914.
- [116] H. Kim, J. Lu, M.S. Sacks, K.B. Chandran, Dynamic simulation of bioprosthetic heart valves using a stress resultant shell model, *Ann. Biomed. Eng.* 36 (2) (2008) 262–275.
- [117] A. Caballero, F. Sulejmani, C. Martin, T. Pham, W. Sun, Evaluation of transcatheter heart valve biomaterials: biomechanical characterization of bovine and porcine pericardium, *J. Mech. Behav. Biomed. Mater.* 75 (2017) 486–494.
- [118] J. Jeong, F. Hussain, On the identification of a vortex, *J. Fluid Mech.* 285 (1995) 69–94.
- [119] B.J. Delemarre, C.A. Visser, H. Bot, A.J. Dunning, Prediction of apical thrombus formation in acute myocardial infarction based on left ventricular spatial flow pattern, *J. Am. Coll. Cardiol.* 15 (2) (1990) 355–360.
- [120] R. Delewi, F. Zijlstra, J.J. Piek, Left ventricular thrombus formation after acute myocardial infarction, *Heart* 98 (23) (2012) 1743–1749.
- [121] M. Li, J.G. Dumesnil, P. Mathieu, P. Pibarot, Impact of valve prosthesis-patient mismatch on pulmonary arterial pressure after mitral valve replacement, *J. Am. Coll. Cardiol.* 45 (7) (2005) 1034–1040.
- [122] J.-F. Ren, S. Aksut, G.W. Lighty Jr, G.J. Vigilante, J.D. Sink, B.L. Segal, W.C. Hargrove, Mitral valve repair is superior to valve replacement for the early preservation of cardiac function: relation of ventricular geometry to function, *Am. Heart J.* 131 (5) (1996) 974–981.
- [123] Y. Okita, S. Miki, K. Kusuhara, Y. Ueda, T. Tahata, K. Yamanaka, T. Higa, Analysis of left ventricular motion after mitral valve replacement with a technique of preservation of all chordae tendineae. comparison with conventional mitral valve replacement or mitral valve repair., *J. Thorac. Cardiovasc. Surg.* 104 (3) (1992) 786–795.
- [124] Z. Popovic, I. Barac, M. Jovic, G. Panic, M. Miric, M. Bojic, Ventricular performance following valve replacement for chronic mitral regurgitation: importance of chordal preservation, *J. Cardiovascular Surgery* 40 (2) (1999) 183–190.
- [125] C.-H. Lee, D.W. Laurence, C.J. Ross, K.E. Kramer, A.R. Babu, E.L. Johnson, M.-C. Hsu, A. Aggarwal, A. Mir, H.M. Burkhart, R.A. Townner, R. Baumwart, Y. Wu, Mechanics of the tricuspid valve—from clinical diagnosis/treatment, in-vivo and in-vitro investigations, to patient-specific biomechanical modeling, *Bioengineering* 6 (2019) 47.
- [126] D.W. Laurence, E.L. Johnson, M.-C. Hsu, R. Baumwart, A. Mir, H.M. Burkhart, G.A. Holzapfel, Y. Wu, C.-H. Lee, A pilot in silico modeling-based study of the pathological effects on the biomechanical function of tricuspid valves, *Int. J. Numer. Method Biomed. Eng.* 36 (2020) e3346.
- [127] M.C.H. Wu, D. Kamensky, C. Wang, A.J. Herrema, F. Xu, M.S. Pigazzini, A. Verma, A.L. Marsden, Y. Bazilevs, M.-C. Hsu, Optimizing fluid–structure interaction systems with immersogeometric analysis and surrogate modeling: application to a hydraulic arresting gear, *Comput. Methods Appl. Mech. Eng.* 316 (2017) 668–693.
- [128] N. Westerhof, J.-W. Lankhaar, B.E. Westerhof, The arterial windkessel, *Med. Biol. Eng. Comput.* 47 (2009) 131–141.