


Protocol

Direct IgG epitope mapping on bacterial AB toxins by cryo-EM

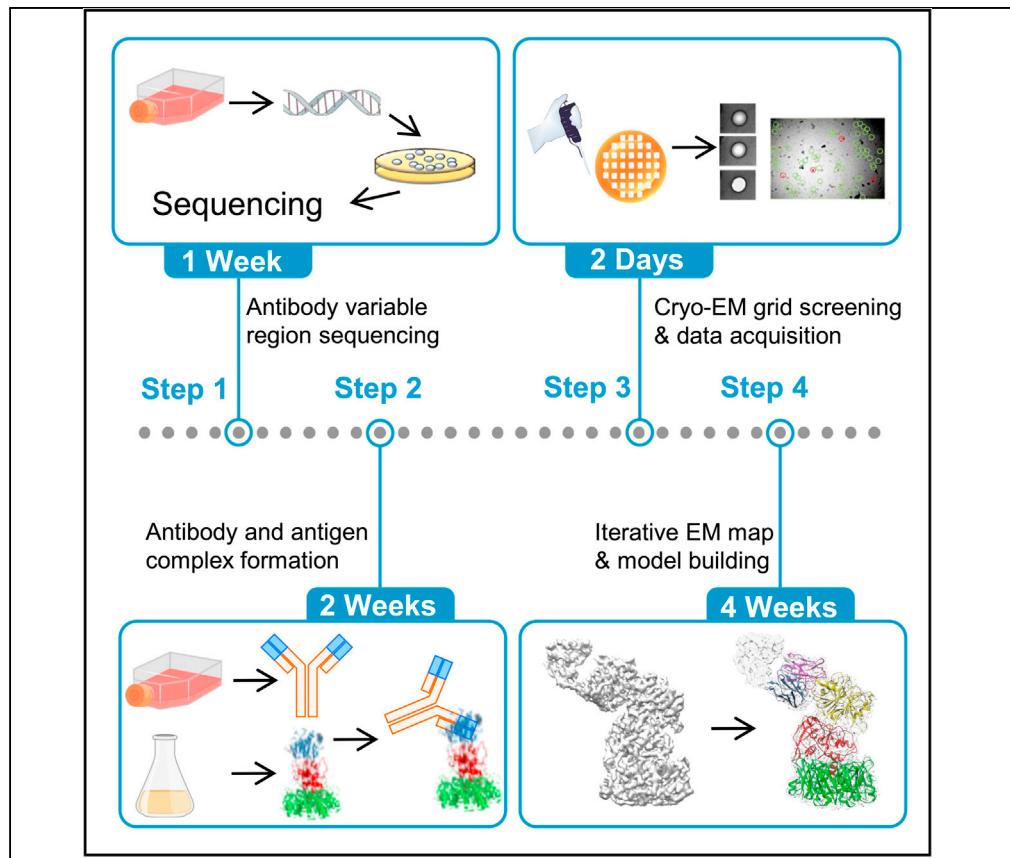

This cryo-EM protocol was used to determine the B cell epitope map on the CdtB subunit of typhoid toxin, an A₂B₅ toxin secreted by *Salmonella Typhi* during infection. Immunoglobulin G (IgG) was directly mixed with typhoid toxin in this protocol, different from our previous cryo-EM protocol that uses the Fab fragments in place of IgG. This simple approach requires smaller amounts of materials, supporting the broader use of this protocol for determining antibody recognition sites on various antigens.

Tri Nguyen,
Jeongmin Song

tn332@cornell.edu (T.N.)
jeongmin.song@cornell.edu (J.S.)

Highlights
This protocol describes the entire procedures for determining antibody target sites

One bacterial AB toxin and toxin-recognizing mAb pair was used as an example

IgG can be directly used to determine the B cell epitope map

This protocol offers insights into other projects concerning mAb-antigen complexes

Nguyen & Song, STAR
Protocols 2, 100852
December 17, 2021 © 2021
The Author(s).
<https://doi.org/10.1016/j.xpro.2021.100852>



Protocol

Direct IgG epitope mapping on bacterial AB toxins by cryo-EM

Tri Nguyen^{1,2,*} and Jeongmin Song^{1,3,*}

¹Department of Microbiology & Immunology, Cornell University, Ithaca, NY 14853, USA

²Technical contact

³Lead contact

*Correspondence: tn332@cornell.edu (T.N.), jeongmin.song@cornell.edu (J.S.)

<https://doi.org/10.1016/j.xpro.2021.100852>

SUMMARY

This cryo-EM protocol was used to determine the B cell epitope map on the CdtB subunit of typhoid toxin, an A₂B₅ toxin secreted by *Salmonella Typhi* during infection. Immunoglobulin G (IgG) was directly mixed with typhoid toxin in this protocol, different from our previous cryo-EM protocol that uses the Fab fragments in place of IgG. This simple approach requires smaller amounts of materials, supporting the broader use of this protocol for determining antibody recognition sites on various antigens.

For complete details on the use and execution of this protocol, please refer to Ahn et al. (2021) and Nguyen et al. (2021).

BEFORE YOU BEGIN

This protocol describes specific steps for determining the B cell epitope map of IgG targeting the CdtB subunit of typhoid toxin.

Buffer preparation

⌚ Timing: 1 day

Antibody purification

1. Binding buffer – Store at 4°C for up to 1 month

Prepare 1 L of the Protein G binding buffer containing 20 mM sodium phosphate, pH 7.0.

2. Elution buffer – Store at 4°C for up to 1 month

Prepare 100 mL of the elution buffer containing 0.1 M glycine-HCl, pH 2.7.

3. Equilibration buffer – Store at 4°C for up to 1 month

Prepare 100 mL of the equilibration buffer containing 1 M Tris-HCl, pH 8.0.

Antigen purification

4. Buffer A – Store at 4°C for up to 1 month

Prepare 200 mL buffer A containing 15 mM Tris-HCl, pH 8.0, 150 mM NaCl, 20 mM imidazole.



Buffer A

Reagent	Final concentration	Amount
1 M Tris-HCl, pH 8.0	15 mM	3 mL
2 M NaCl	150 mM	15 mL
Imidazole	20 mM	0.27 g
ddH ₂ O	n/a	Make up the volume 200 mL with ddH ₂ O
Total	n/a	200 mL

Store at 4°C for up to 1 month

5. Buffer B – Store at 4°C for up to 1 month

Prepare 50 mL buffer B containing 20 mM Tris-HCl, pH 8.0, 200 mM NaCl, 300 mM imidazole.

Buffer B

Reagent	Final concentration	Amount
1 M Tris-HCl, pH 8.0	20 mM	1 mL
2 M NaCl	200 mM	5 mL
Imidazole	300 mM	1.02 g
ddH ₂ O	n/a	Make up the volume 50 mL with ddH ₂ O
Total	n/a	50 mL

Store at 4°C for up to 1 month

6. Buffer C – Store at 4°C for up to 1 month

Prepare 1 L buffer C containing 10 mM 2-(N-morpholino)ethanesulfonic acid (MES), pH 6.0.

7. Buffer D – Store at 4°C for up to 1 month

Prepare 500 mL buffer D containing 10 mM MES, pH 6.0, 1 M NaCl.

8. Buffer E – Store at 4°C for up to 1 month

Prepare 500 mL buffer E containing 15 mM Tris-HCl, pH 8.0, 150 mM NaCl.

Antibody-antigen complex preparation

9. Buffer F – Store at 4°C for up to 1 month

Prepare 1 L buffer F containing 15 mM Tris-HCl, pH 7.5 and 150 mM NaCl.

⚠ CRITICAL: When you make buffers, add only 75% of H₂O and let the buffer cool for at least 18 hours at 4°C before adjusting pH.

KEY RESOURCES TABLE

REAGENT or RESOURCE	SOURCE	IDENTIFIER
Chemicals, peptides, and recombinant proteins		
Imidazole	Sigma	I0125
IPTG, Dioxane-Free	Thermo Fisher	R0393

(Continued on next page)

Continued

REAGENT or RESOURCE	SOURCE	IDENTIFIER
Pierce Protease Inhibitor Tablet, EDTA-free	Thermo Fisher	A32965
Lysozyme from chicken egg white	Sigma	L6876
DNase I	Alfa Aesar	J62229
PROTEININDEX HiBond Ni-NTA Agarose 6 Fastflow	Marvelgent	11-0225-010
XK16/20 column	GE Scientific	28988937
HiTrap SP HP	Cytiva	17-1152-01
SD200 10/300GL Increase columns	Cytiva	28-9909-44
Pierce NHS-Activated Agarose	Thermo Fisher	26200
Bradford reagent	Bio-Rad	5000006
Amicon Ultra-15 30 kDa cutoff	Millipore	UFC903024
Critical commercial assays		
RNeasy Mini Kit	QIAGEN	74104
iScript cDNA Synthesis Kit	Bio-Rad Laboratories	1708891
Herculase II Fusion DNA polymerase	Agilent	600677
Phusion DNA polymerase	New England Biolabs	M0530
QIAEX II DNA Extraction Kit	QIAGEN	20021
Deposited data		
Typhoid toxin bound to TyTx11 MAb	RCSB Protein Data Bank	PDB ID of 6VX4
Typhoid toxin bound to TyTx1 and TyTx4 Fab	RCSB Protein Data Bank	PDB ID of 7K7H and 7K7I
Experimental models: Cell lines		
Hybridomas	(Ahn et al., 2021; Nguyen et al., 2021)	See Methods Details of the referred papers
Oligonucleotides		
See Table 1	Integrated DNA Technologies (IDT)	Table 1
Software and algorithms		
Unicorn 6.3	GE Healthcare Life Sciences	https://www.gelifesciences.com/en/us/shop/unicorn-6-3-p-01118
CryoSparc 2	(Punjani et al., 2017)	https://cryosparc.com
Relion 3	(Zivanov et al., 2018)	https://www3.mrc-lmb.cam.ac.uk/relion/index.php/Main_Page
PyMol	Schrodinger	https://pymol.org/2/
Chimera	UCSF Chimera	https://www.cgl.ucsf.edu/chimera/
PHENIX	(Adams et al., 2010)	https://www.phenix-online.org/
Coot	(Emsley et al., 2010)	https://www2.mrc-lmb.cam.ac.uk/personal/pemsley/coot/

STEP-BY-STEP METHOD DETAILS

Below we provide a step-by-step protocol describing the sequencing of antibody variable regions, purification of antibody and antigen, and structure determination of the antibody-antigen complex (Figure 1).

Antibody variable region sequencing

⌚ Timing: 1 week

This step allows for the accurate determination of the amino acid sequences of the variable regions of the heavy and light chains of the antibody. These sequences are vital for the atomic structural model building and fitting into the electron density data from cryo-EM analyses. The antibody variable region sequencing protocol was adopted from (Meyer et al., 2019).

1. Total RNA was extracted from the hybridoma cells using the RNeasy mini kit by following the vendor's recommendations (Qiagen).

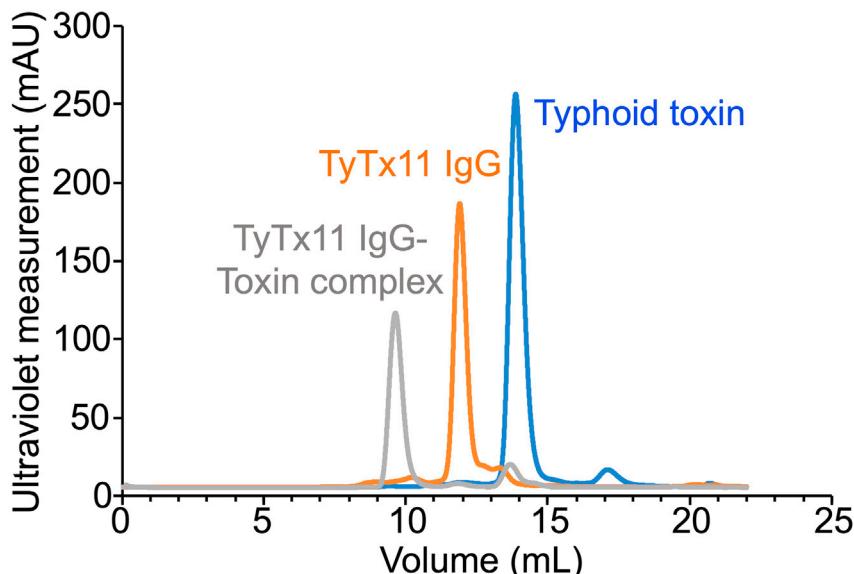


Figure 1. Typical size-exclusion chromatograms showing antibody only (orange line), antigen only (blue line), and antibody-antigen complex (gray line).

2. cDNA synthesis was performed using the iScript cDNA synthesis system (Bio-Rad) with the mouse IgG reverse transcription primers listed in [Table 1](#). The reaction condition is listed in [Table 2](#).
3. To amplify the antibody variable regions from the cDNA, a two-stage PCR reaction ([Tables 3](#) and [4](#)) was run with the universal forward PCR primer and reverse PCR primer based on the antibody chain ([Table 1](#)).
4. The amplicons from the 1st PCR reaction ([Table 3](#)) appeared between 550–600 base pairs on 1 % agarose gel.
5. The amplicon DNA was extracted from the gel using the QIAEX II DNA Extraction Kit by following the vendor's recommendations (Qiagen).
6. The extracted DNA was used to set up the 2nd-stage PCR ([Table 4](#)). The PCR amplicon was extracted and Gibson-assembled to the pET28a⁺ plasmid (EMD Biosciences). The pET28a⁺ vector amplicon was prepared using the primer pair matching the light and heavy chains ([Tables 1](#) and [4](#)).
7. The Gibson-assembled circular plasmid was transformed into *E. coli* DH5 α , a single colony was isolated, and the isolated plasmid was Sanger-sequenced using either T7 promoter or T7 terminator primer ([Table 1](#)).

Note: Other plasmids and *E. coli* strains can be used.

⚠ CRITICAL: The PCR amplicons could be directly sequenced to determine the antibody variable regions via Sanger sequencing. However, we found out that the sequencing outcomes were less satisfactory and counter-productive due to ambiguous base calls in our cases.

Purification of antibody

⌚ Timing: 1 week

8. Cell culture supernatants of the hybridomas generated as part of ([Ahn et al., 2021](#); [Nguyen et al., 2021](#)) were prepared by centrifugation for 15 min at approximately 6,000 \times g at 4°C using JLA8.1 rotor, followed by filtration through 0.2 μ m cellulose acetate filters.

Table 1. Primer sequences used in this study

Application	Primer name	Forward or reverse	Primer sequence (5'-3')
Reverse transcription (Meyer et al., 2019)	Template-switch oligo	Universal forward	AGGCAGTGGTATCAACGCAGACTACAT GrGrGr (GrGrGr: 3 riboguanines)
	mIGK RT	Kappa chain reverse	TTGTCGTTCACTGCCATCAATC
	mIGL RT	Lambda chain reverse	GGGGTACCATCTACCTTCCAG
	mIGH RT	Heavy chain reverse	AGCTGGAAAGGTGTCACAC
PCR (Meyer et al., 2019)	ISPCR	Universal forward	AAGCAGTGGTATCAACGCAGAG
	mIGK PCR	Kappa chain reverse	ACATTGATGTTGGGTAGAAG
	mIGL PCR	Lambda chain reverse	ATCGTACACACCAGTGTGGC
	mIGH PCR	Heavy chain reverse	GGGATCCAGAGTTCCAGGTC
Gibson assembly	pET-F	Forward	CTCTGCGTTGATACCACTGCTTGATCCG GCTGCTAAC
	pET-R for kappa chain	Reverse	CTTCTACCCCAAAGACATCAATGTCATGG TATATCTCTTC
	pET-R for lambda chain	Reverse	GCCACACTGGTGTACGATCATGGTA TATCTCTTC
	pET-R for heavy chain	Reverse	GACCTGGAACTCTGGATCCCCATGGTA TATCTCTTC
Sequencing	T7 promoter	Forward	TAATAGCACTCACTATAGGG
	T7 terminator	Reverse	GCTAGTTATTGCTCAGCGG

9. Protein G resins were packed in a 25 mL gravity plastic column and equilibrated by flowing 20 mL of the binding buffer (20 mM sodium phosphate buffer, pH 7.0).
10. The cleared hybridoma supernatants from step 8 were submitted to the prepared Protein G resin from step 9 three times.
11. The antibody-bound resins were washed with 25–50 mL of the binding buffer.
12. The bound antibodies were eluted by applying 10 mL of the elution buffer (0.1 M glycine-HCl, pH 2.7), which was harvested in a conical tube containing 1 mL of the equilibration buffer (1 M Tris-HCl, pH 8.0) for immediate neutralization.
13. The purity and yield of purified antibodies were monitored via 15% SDS-PAGE.
14. Purified antibodies were divided in 50 µL aliquots and stored at –80°C until use.

Note: Flash freezing with liquid nitrogen was not required in this case. Purified antibodies were stored stably without excipients such as glycerol. However, if desired, flash freezing and the addition of excipients like glycerol can be considered in this step.

Optional: IgG was directly used for the complex structure determination for TyTx11 mAb (Ahn et al., 2021). However, if desired, the following steps can be carried out to prepare the Fab fragment, as described in (Nguyen et al., 2021).

15. Fab fragment generation:
 - a. Concentrate purified mAbs to 20 mg/mL in 0.1 mL of a buffer containing 20 mM sodium phosphate, pH 7.0, and 10 mM EDTA.
 - b. Mix 250 µL of equilibrated immobilized Papain (ThermoFisher) with 1 mL of concentrated mAbs and incubate for at least 16 h at 37°C.
 - c. Elute the digested mAb samples in a buffer containing 10 mM Tris-HCl, pH 7.5.
 - d. Separate the Fab from uncut mAbs and the Fc by carrying out using a Superdex 75 10/300 Increase column (GE Healthcare) with a buffer containing 10 mM Tris-HCl, pH 7.5 at a constant flow of 0.5 mL/min.

Purification of typhoid toxin (antigen)

⌚ Timing: 3 days

Table 2. cDNA synthesis reaction

Steps	Temperature	Time	Cycles
Priming	25°C	5 min	1
Reverse transcription	42°C	60 min	1
RT Inactivation	95°C	1 min	1
Hold	4°C	Forever	

A highly purified antigen is vital for the generation and purification of the antigen-antibody complex. The uniformity of antigen and subsequent antigen-antibody complex improves the quality and reproducibility of data obtained during cryo-EM analysis.

16. Three subunits of typhoid toxin, PltB, PltA, and CdtB, were cloned together into pET28a⁺ with a C-terminal His₆ tag (Song et al., 2013).

Note: The in-frame ORFs of PltB and PltA were cloned downstream of a T7 promoter provided by pET28a⁺. The ORF for CdtB was added downstream of PltB and PltA to be in-frame with the C-terminal His₆ tag presented on pET28a⁺. This design allowed for the expression of all three genes by the induction of T7 promoter.

17. Preparing bacterial cell pellet:

- Transform the typhoid toxin plasmid in *E. coli* BL21(DE3) competent cells.
- Pick, inoculate, and culture a single colony in 10 mL of LB for at least 18 h at 37°C in a glass culture tube.
- The next day, transfer 5 mL of the 10 mL bacterial culture into 50 mL of LB in a 250-mL baffled flask.
- After 3 h of culture at 37°C, transfer 10 mL of this culture to each 1 L of LB in a 2-L baffled flask and continue to culture at 37°C, 200 rpm for 1.5–2 h.
- When OD₆₀₀ reaches 0.5, change the setting to 28°C and 130 rpm.
- After 30 min, add 250 µL of 0.5 M isopropyl β-D-1-thiogalactopyranoside (IPTG) to each culture (final concentration, 125 µM) and stir before placing the culture back to the incubator for 17–18 h.
- Harvest the bacterial cells in a 1 L centrifuge bottle with 5000 × g for 15 min at 4°C.
- Pour off the supernatant into an empty flask and bleached (10% v/v) to discard.

Note: If desired, scoop out the pellet and combine up to 2 flasks worth of pellets into a single 50 mL tube.

- Store the pellet at –80°C if desired.

18. Bacteria lysis and centrifugal clarification:

- In a 50 mL conical tube containing bacterial pellets from up to 2 L culture, add 25 mL of buffer A and vortex to resuspend.
- Add a protease inhibitor cocktail solution (final, 1x), 2 mg/mL of lysozyme, and 40 µg/mL of DNase I and invert the tube several time to mix.
- Subject the bacteria solution to 3 repeats of freeze-thaw in liquid nitrogen.
- Lyse the cells using a 200-Watt ultrasonic homogenizer with a 1/8" probe (VWR).
- Use the 'Time – Pulse' setup with the 75% power, 20 sec-on, and 20 sec-off for 4 min.
- Clarify the lysate by centrifugation for 30 min at 18,000 × g at 4°C.

19. Ni-Immobilized Metal Affinity chromatography (IMAC):

- Load the clarified lysate onto 10 mL of Ni-NTA equilibrated with buffer A.
- Wash the column with 100 mL of buffer A.
- Elute the protein with 50 mL of buffer B and collect 7 mL fractions.

Table 3. 1st-stage PCR amplification of the antibody variable region

Steps	Temperature	Time	Cycles
Initial Denaturation	98°C	30 s	1
Denaturation	98°C	15 s	10 cycles
Annealing	55°C	30 s	
Extension	72°C	30 s	
Final extension	72°C	5 min	1
Hold	4°C	Forever	

d. Combine elute fractions containing desired protein and concentrate using Amicon columns, 30 kDa cutoff (ThermoFisher) until the volume reaches less than 5 mL.

20. HiTrap SP HP cation exchange chromatography:

- In a 50 mL conical tube, add 45 mL of buffer C and up to 5 mL of the concentrated Ni-IMAC eluate to lower the pH and salt level.
- Load the protein solution onto a 5 mL SP HiTrap column equilibrated with buffer C.
- Connect the column to the AKTA system.
- Run the 'Toxin SP – Opt (or any name that you prefer to use)' program:
AKTA A-line equilibrated with buffer C, B-line equilibrated with buffer D.
 - A flow rate of 1 mL/min.
 - Fractionation of 1 mL for 60 mL.
 - Gradient going from 0 to 40% buffer D for 50 mL.
 - At 50 mL, gradient going from 40% to 100% for 1 mL.
 - At 70 mL, gradient going from 100% to 0% for 1 mL.
 - At 90 mL, stop method.
- Run SDS-PAGE of the fractions containing UV-peaks to identify the fractions of interest.
- Pool the fractions containing the toxin and concentrate using a 5 mL Amicon column, 30 kDa cutoff, by spinning at 3500 × g for ~15 min at 4°C until the volume reaches 400–500 µL.

21. Size Exclusion Chromatography:

Optional: PBS can be used in place of buffer E if the downstream procedure is not compatible with Tris.

- Equilibrate a Superdex 200 10/300GL increase column with buffer E.
- Load the concentrated protein elute from the HiTrap SP chromatography (up to 500 µL) through the manual injection port of AKTA into the 500 µL sample loop.
- Run the 'Size Ex – 500 µL (or any name that you prefer to use)' program:
AKTA A-line equilibrated with buffer E
 - A flow rate of 0.25 mL/min.
 - Fractionation of 0.5 mL for 28 mL.
 - Inject 0.5 mL from the 500 µL sample loop (Cytiva).
 - At 28 mL, stop method.

Note: In the case of typhoid toxin, you should see the UV peak around 12 mL–14.5 mL, which equates to an estimate of 110–120 kDa.

- Aliquot the toxin and freeze at –80°C until use.
- Assess the toxin concentration and analyze on SDS-PAGE.

Note: Western blot and/or mass spectrometry can be carried out if further validation is desired.

Table 4. 2nd-stage PCR reactions for the antibody variable region and vector

Steps	Temperature	Time	Cycles
Initial Denaturation	98°C	2 min	1
Denaturation	98°C	20 s	35 cycles
Annealing	55°C	20 s	
Extension	72°C	1 min for insert, 3 min for vector	
Final extension	72°C	5 min	1
Hold	4°C	Forever	

Optional: If the antibody recognition site overlaps with the location of the tag used for protein purification, the tagless version of proteins can be prepared. The following is the procedure that we used to obtain the tagless typhoid toxin (Nguyen et al., 2021).

22. Preparation of a column packed with the TyTx1 antibody-conjugated agarose resin:

- Transfer 1 mL of the settled Pierce NHS-activated agarose resin (ThermoFisher, cat# 26200), wash with PBS, and incubate with PBS containing 14 mg of the TyTx1 antibody (Nguyen et al., 2021) for 1 h at 25°C with gentle rocking for the conjugation to occur.
- Wash the resin four times with 5 mL of PBS.
- Quench the resin by repeated washing with 10 mL of 0.5 M Tris-HCl, pH 8.0, and store at 4°C until use.

Note: The resin should be stable for longer than a year. Proper handling of the resin including buffer selection and cleaning will ensure a long shelf-life of the resin.

23. Purification of the tagless typhoid toxin:

- Culture *E. coli* BL21(DE3) harboring pET28a⁺ carrying tagless typhoid toxin subunits in LB to approximately OD₆₀₀=0.7 at 37°C, transfer to 28°C, add with 0.5 mM IPTG, and incubate for 16 h.
- Resuspend the harvested bacteria pellet in buffer E containing 1x EDTA-free protease inhibitor cocktail, 0.2 mg/mL lysozyme, and 80 µg/mL DNase I, and subject to 3 times of the freeze-thaw step in liquid nitrogen, and lyse the bacterial cells by sonication. See steps 17–18 for details.
- Clarify the lysate by centrifugation at 18,000 × g for 30 min at 4°C.
- Mix the clarified lysate with the prepared TyTx1-conjugated agarose and incubate at 4°C for 30 min with gentle rocking.
- Recapture the resin by passing the lysate through a gravity column and wash with buffer E.
- Elute the protein with 5 mL of 100 mM Glycine, pH 3.0, and quickly neutralize the eluted protein by adding 1 mL of 1 M Tris-HCl, pH 8.8.
- Apply the purified protein to size exclusion chromatography.

Antibody-antigen complex and cryo-EM grid preparation

⌚ Timing: 1 day

24. Antibody-antigen complex preparation:

- Prepare TyTx11 mAbs bound to wild-type purified typhoid toxin (PltB, PltA, CdtB) by at least 16 h incubation of the 1:1 mixture of antibody and toxin (250 µL each of ~1.2 mg/mL proteins) at 4°C.
- Submit the antibody-antigen mixture to a Superdex 200 10/300 increase column (Cytiva) using a constant flow of 0.5 mL/min of buffer F (15 mM Tris-HCl, pH 7.5 and 150 mM NaCl).

- c. Collect fractions corresponding to the antibody-antigen complex ([Figure 1](#)). Measure the concentrations using the Bradford solution (Bio-Rad, cat# 5000006) and use the purified complexes immediately for Cryo-EM grid/sample preparations using buffer F.

25. Grid preparation:

- a. Dilute IgG-toxin complex samples with buffer F to a final concentration of 0.1 and 0.2 mg/mL providing a variable for grid screening.
- b. Apply samples (3.5 μ L) to glow-discharged copper Quantifoil R1.2/1.3 300 mesh cryo-EM grid (EMS) mounted, blotted, and plunge frozen in liquid ethane using a Vitrobot (ThermoFisher) at 100% humidity at 4°C.
 - i. One of the common settings for Vitrobot was: Blot total – 1; Blot force – 1; Blot time – 2 to 4 s; Drain time – 1 s; Wait time – 0 s.
- c. Store frozen grids in liquid nitrogen until analysis.

Cryo-EM grid screening and data acquisition

⌚ Timing: 1 day

26. Grid Screening:

- a. Test two variables per antibody-toxin complex: blot times and protein concentrations.

Note: Optimal protein concentrations and blot times may vary depending on samples, which can be empirically determined. As shown in [Figure 2](#), good grids should have wells containing thin vitrified ice with good protein complex dispersal. In our case, using two different protein concentrations, 0.1 mg/mL and 0.2 mg/mL, we tested 4 different blot times: 2.5, 3, 3.5 and 4s to screen for good grid, resulting in 8 different grids. The initial screen indicated that a concentration of 0.1 mg/mL was suitable for imaging.

27. Data Acquisition:

- a. In our case, data were acquired at a nominal magnification of 63,000 \times for TyTx11 using a Talos Arctica (ThermoFisher) operating at 200 kV equipped with a Gatan energy filter set to a slit width of 20 eV and K3 detector operating in super-resolution counting mode using a defocus range of –0.8 to –1.8 μ m.
- b. In our case, 50 frame movies with a super-resolution pixel size of 1.23 were collected over a 4-s exposure, resulting in a total dose of 54.7 $e^- \text{ \AA}^{-2}$ (1.06 $e^- \text{ \AA}^{-2}$ /frame) for the TyTx11/Toxin complex.

Note: To provide an example, in the case of our TyTx1 and TyTx4 study, we took approximately 150–200 movies that successfully yielded the complex structures for TyTx1 and TyTx4 ([Nguyen et al., 2021](#)).

Note: A newer software like CryoSparc Live processes images captured by camera real-time, informing the researcher when to stop.

Cryo-EM data processing

⌚ Timing: 2–3 weeks

The simplified version of the cryo-EM data processing workflow is shown in [Figure 3](#). See Ahn et al. ([Ahn et al., 2021](#)) for additional details.

28. Image import, motion correction, and contrast transfer function (CTF) estimation:

- a. Perform motion correction of each image stack using MotionCor2 function in RELION ([Zheng et al., 2017](#); [Nakane et al., 2018](#)).

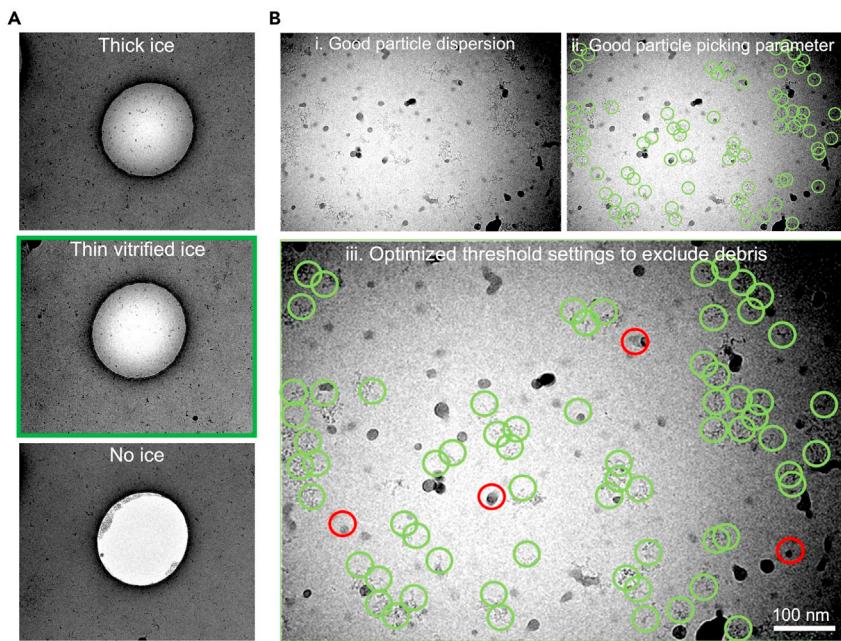


Figure 2. Cryo-EM sample and grid preparation

Examples of good and bad ice.

(A) The panel in the middle (thin vitrified ice) is a good example that typically shows protein particles with suitable dispersion.
 (B) Samples with thin vitrified ice were examined for particle dispersion and marked for data collection (i). During data processing, suitable particle picking parameters were set to auto-pick most particles (ii). Subsequent rounds of particle picking were carried out to exclude non-protein debris particles (iii).

- b. Following CTF estimation by CTFFIND-4.1 via Relion 3, subject the movies (i.e., a total of 935 movies collected during data acquisition) to Laplacian-of-Gaussian particle picking in RELION 3.
29. Approximately 1000 particles were manually picked, extracted, and 2D classified to serve as initial templates for automated particle picking in RELION 3.
30. The resulting 1,009,626 particles were extracted at 3.0457 Å/pixel to reduce the memory requirements during computation and to speed up image processing (Figure 3).
31. The 2D classification was used to remove incorrectly picked particles (Figure 3 left panel).
32. CryoSparc 2 was used to generate an 3D ab initio model from the cleaned particle set.
33. This 3D ab initio model was used as a reference map for subsequent 3D classifications and refinement in RELION 3.
34. Initial 3D classification revealed three out of five classes containing particles resembling the structure of Fab (Figure 3 right panel).
35. The particles from those classes were combined and submitted to another round of 3D classification, which revealed one of four classes contained high-quality particles resulting in a high-resolution estimate for the model (Figure 3 middle-right panel).
36. Particles from this class were then used for subsequent per-particle CTF refinements and 3D refinement (Figure 3 bottom-right panel).
37. When no further improvement could be made, the particles were then un-binned and re-extracted at 1.23 Å/pixel.
38. After subsequent CTF refinements and 3D refinements, a Bayesian polishing step followed by a final 3D classification was used to remove any last junk particles.
39. Final reconstruction using 61,478 particles was generated. The final 3D reconstruction has a 0.143 FSC cutoff resolution of 3.12 Å according to RELION3 (Figure 43 bottom left panel).

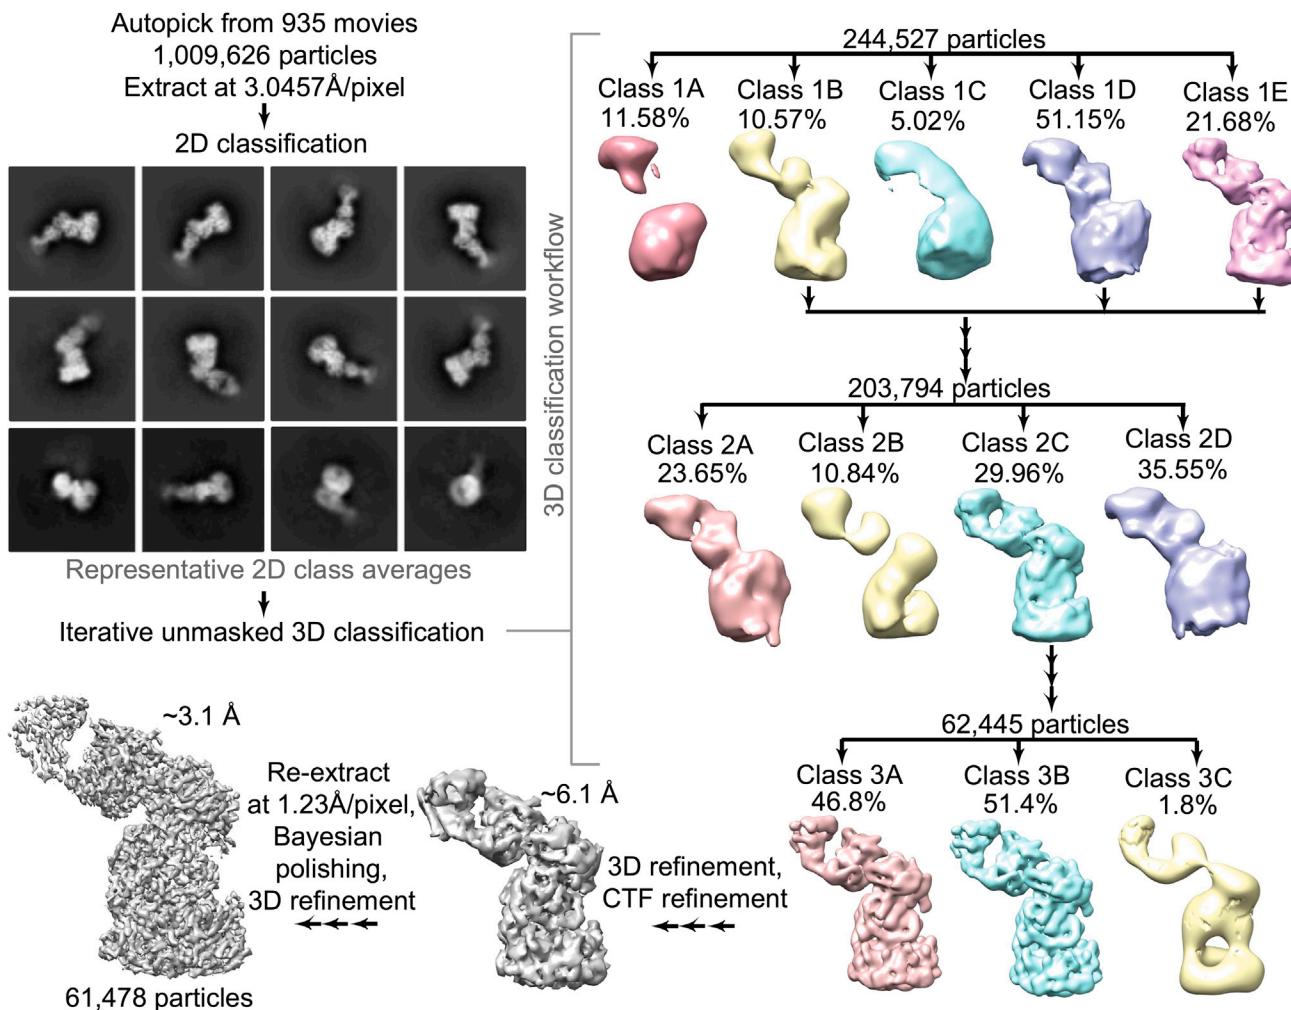


Figure 3. Typical workflow of cryo-EM data processing

See also Ahn et al. (Ahn et al., 2021) for 2D classification and other details.

Structural model building

⌚ Timing: 1 week

40. Chimera (www.cgl.ucsf.edu) was used to place the crystal structures of typhoid toxin (PDB 4K6L) and PltB pentamer (PDB 4RHR) into the sharpened reconstructions as preliminary atomic models. See Ahn et al. (Ahn et al., 2021) for additional details.
41. The preliminary atomic models for TyTx11 Fab variable region were obtained from the following models selected based on sequence similarity through BLAST: the light chain from PDB 6GFF and the heavy chain from PDB 1F11. The constant regions of the TyTx11 were too flexible for the proper density fitting and thus left unbuilt in the final deposited model.
42. Coot (www.biop.ox.ac.uk/coot) was then used to manually rebuild these preliminary models. The flexibility of the antibody constant regions, CdtB subunit, and the majority of the PltA subunit prevented us from confidently building these portions of the maps, so they were left unbuilt.
43. Cyclical refinement step involving model manually modified in Coot was submitted to automated real-space refinement in Phenix (phenix-online.org), which was manually modified in

Coot to lower clashes and fix outliers. The quality of the final models was validated using MolProbity (molprobity.biochem.duke.edu).

44. Figures were generated using Chimera and Pymol (Schrodinger, Inc). Cryo-EM density maps and refined complex structures were deposited under EMD-21429 and PDB 6VX4 for the TyTx11 MAb-toxin complex.

EXPECTED OUTCOMES

Here, we have described step-by-step experimental procedures that we used to obtain the sequences of antibody variable regions, purifications of antibody and antigen, and structure determination of the antibody-antigen complex. This protocol provides practical insights into other projects aimed at solving the structures of the antibody and bacterial toxin complexes.

LIMITATIONS

Obtaining ultrapure antibodies and antigens will be vital to high-resolution B cell epitope mapping of antibodies. The uniformity of antigen and subsequent antigen-antibody complexes will also be critical to the quality and reproducibility of data obtained during cryo-EM analysis.

TROUBLESHOOTING

Problem 1

The direct use of IgG has several advantages such as the requirement of smaller amounts of materials, less time and labor. Also note that in some cases that need to be determined empirically, the use of IgG is required as the Fab fragment is not stable. In addition, the use of IgG can improve the signal contrast for particle picking and help avoid orientation bias among particle groups. Conversely, the use of the Fab fragment can be required for some cases and therefore the use of Fabs and IgG can be empirically determined depending on the experimental needs and the questions to address.

In step 24, if the direct use of IgG is not suitable for yielding reliable antigen-antibody complexes, the Fab fragments can be prepared and used in place of IgG.

Potential solution

Detailed procedures relevant to obtaining the Fab fragments are described in step 15 using two antibodies, TyTx1 and TyTx4, as examples.

Problem 2

In step 24, the hexahistidine tag used for antigen purification might be located on/near the epitope recognized by the antibody. Standard ELISA can address whether the tag location and amino acid residues recognized by the antibody overlap.

Potential solution

Suppose the antibody recognition site overlaps with the location of the epitope tag used for protein purification. In that case, it can be resolved by preparing the tagless version of proteins or relocating the tag to somewhere else on the antigen.

Problem 3

In step 4, the PCR amplicons could be directly sequenced in antibody sequencing to determine the antibody variable regions via Sanger sequencing. However, the direct sequencing of PCR amplicons might yield unsatisfactory outcomes.

Potential solution

As described in steps 6–7, PCR amplicons can be inserted into a plasmid before sequencing the antibody variable region.

Problem 4

In step 26, the grids screening variables might not yield any good grids.

Potential solution

Good grids and subsequent good dataset can be varied from proteins to proteins. Depending on the size of the protein complex, protein concentrations can be altered for better particle dispersions. Other factors to optimize include tweezer handling of grids, awareness of cryogenic fluids throughout the preparation steps, and careful transfer of grids to cryo-EM machine. Seasonal awareness of humidity can also help optimize blot-time for ice formation.

Problem 5

In step 29, during particle picking, depending on the proteins, a large portion of particles can appear clumping in large patches in the micrographs and therefore the number of single particles appear to be insufficient for picking.

Potential solution

Instead of picking only isolated single particles, both isolated single particles and particles found in clump patches can be used by performing the following steps. Both types of particles are picked manually, followed by automated picks using a 2D template generated by the initial manual picks. For instance, after picking around 1,000 particles from different defocus, a 2D template can be generated and served a guide for automated particle picks. 2D and 3D classification will improve the signal to noise ratio in the particles found in clumps.

RESOURCE AVAILABILITY

Lead contact

Further information and requests for resources and reagents should be directed to and will be fulfilled by the lead contact, Jeongmin Song (jeongmin.song@cornell.edu).

Materials availability

Unique and stable reagents generated as part of this study are available upon request via an appropriate material transfer agreement.

Data and code availability

The cryo-EM map included in this study has been deposited in the Electron Microscopy Data Bank with accession code: EMD-21429. The atomic coordinate of TyTx11 bound to typhoid toxin has been deposited in the RCSB Protein Data Bank under PDB ID: 6VX4. The cryo-EM maps of TyTx1 and TyTx4 bound to typhoid toxin, where we used the Fab fragments in place of IgG, have also been deposited in the EMDB with accession codes: EMD-22699 and EMD-22700. The atomic coordinates have been deposited in the PDB ID: 7K7H and 7K7I.

ACKNOWLEDGMENTS

We thank Nicholas J. Mantis, Angelene F. Richards, and Greta Van Slyke for the generation and characterization of the hybridomas producing anti-PltB or anti-CdtB antibodies; J. Christopher Fromme and J. Ryan Feathers for their inputs on cryo-EM data analysis; and Mariena S. Ramos and Katie Spoth of the Cornell Center for Material Research (CCMR) for their assistance in using FEI Vitrobot and Talos Artica S/TEM. This study was supported in part by a multi-PI R03 award from NIAID (AI135767) to J.S. and N.J.M.; NIH R01 AI137345, AI139625, and AI141514 to J.S.; and NSF DMR-1719875 to the CCMR. The funders had no role in the study design, data collection, analysis, decision to publish, or manuscript preparation.

AUTHOR CONTRIBUTIONS

T.N. conducted the experiment relevant to the procedures described in this protocol. J.S. and T.N. wrote the manuscript.

DECLARATION OF INTERESTS

The authors declare no competing interests.

REFERENCES

Adams, P.D., Afonine, P.V., Bunkoczi, G., Chen, V.B., Davis, I.W., Echols, N., Head, J.J., Hung, L.W., Kapral, G.J., Grosse-Kunstleve, R.W., et al. (2010). PHENIX: a comprehensive Python-based system for macromolecular structure solution. *Acta Crystallogr. D Biol. Crystallogr.* **66**, 213–221.

Ahn, C., Yang, Y.-A., Neupane, D.P., Nguyen, T., Richards, A.F., Sim, J.H., Mantis, N.J., and Song, J. (2021). Mechanisms of typhoid toxin neutralization by antibodies targeting glycan receptor binding and nuclelease subunits. *iScience* **24**, 102454.

Emsley, P., Lohkamp, B., Scott, W.G., and Cowtan, K. (2010). Features and development of Coot. *Acta Crystallogr. D Biol. Crystallogr.* **66**, 486–501.

Meyer, L., Lopez, T., Espinosa, R., Arias, C.F., Vollmers, C., and Dubois, R.M. (2019). A simplified workflow for monoclonal antibody sequencing. *PLoS One* **14**, e0218717.

Nakane, T., Kimanius, D., Lindahl, E., and Scheres, S.H. (2018). Characterisation of molecular motions in cryo-EM single-particle data by multi-body refinement in RELION. *Elife* **7**, e36861.

Nguyen, T., Richards, A.F., Neupane, D.P., Feathers, J.R., Yang, Y.A., Sim, J.H., Byun, H., Lee, S., Ahn, C., Van Slyke, G., Fromme, J.C., Mantis, N.J., and Song, J. (2021). The structural basis of *Salmonella* A2B5 toxin neutralization by antibodies targeting the glycan-receptor binding subunits. *Cell Rep.* **36**. <https://doi.org/10.1016/j.celrep.2021.109654>.

Punjani, A., Rubinstein, J.L., Fleet, D.J., and Brubaker, M.A. (2017). cryoSPARC: algorithms for rapid unsupervised cryo-EM structure determination. *Nat. Methods* **14**, 290.

Song, J., Gao, X., and Galan, J.E. (2013). Structure and function of the *Salmonella Typhi* chimaeric A(2) B(5) typhoid toxin. *Nature* **499**, 350–354.

Zheng, S.Q., Palovcak, E., Armache, J.P., Verba, K.A., Cheng, Y., and Agard, D.A. (2017). MotionCor2: anisotropic correction of beam-induced motion for improved cryo-electron microscopy. *Nat. Methods* **14**, 331–332.

Zivanov, J., Nakane, T., Forsberg, B.O., Kimanius, D., Hagen, W.J., Lindahl, E., and Scheres, S.H. (2018). New tools for automated high-resolution cryo-EM structure determination in RELION-3. *Elife* **7**, e42166.