

Ultrasonic vs. Magnetic Resonance Communication for Mixed Wearable and Implanted Devices

Rajpreet K Gulati Walia*, Krishna Kant*, Amitangshu Pal†

*Computer and Information Sciences, Temple University, Philadelphia, PA 19122, USA

†Computer Science and Engineering, Indian Institute of Technology Kanpur, Kanpur, India

Abstract—Human body communication (HBC) has recently been explored extensively both for small wearable electronic gadgets and for implanted sensors to deliver relevant data to implanted therapeutic devices. In this paper, we conduct an experimental comparison of two of the promising technologies but for on-body use, namely ultrasound coupling (USC) and magnetic resonance coupling (MRC) based communications. We find that both of these propagate much better through the body than in the air, thereby making them attractive for communications between in-body nodes, in-body to on-body nodes, and on-body nodes where the direct path includes substantial body area. USC also involves a surface acoustic wave (SAW) between on-body nodes which may be broken to varying extent by clothing. We find that with SAW component, USC works better than MRC, but otherwise has similar performance. MRC is very robust and can travel up to the entire body length with 25dB or less loss.

Index Terms—Magnetic resonance coupling; magnetic communication; intra-body sensor network; wireless power transfer

I. INTRODUCTION

A. Motivation and background

Small electronic devices with smart sensing and communications continue to proliferate both for on-body and in-body use. The former, often described as *wearable computing devices* [1], are being used for an increasing array of assistive functions, the most basic ones being those that contact the body and measure some physiological parameters (e.g., temperature, blood pressure, etc.). The devices may also help augment or enhance human sensing capabilities (e.g., smart glasses or smart hearing aids). They may also be more intrusive and provide stimulus or medication in response to the sensed conditions. Implanted devices often perform all of these functions for dealing with chronic illnesses that continue to increase in an aging population in the USA and elsewhere [2].

Although some of these devices can be self-contained, there is a compelling reason for networking these devices together, so that each can do its local function of sensing/actuation in the most energy-efficient manner, and the complexities of combining multiple signals and decision-making can be left to a more capable device. There are already several examples of such a need, such as bladder control and others [3], [4] where signals from several parts around the bladder must be collected and analyzed to determine the electrical stimulation or drug release amounts. A wearable device such as a smart-watch (or a similar form-factor device attached at a suitable point on the body) can be used as a centralized hub for decision-making based on signals from both on-body and in-body devices. The key advantages of an on-body device are high

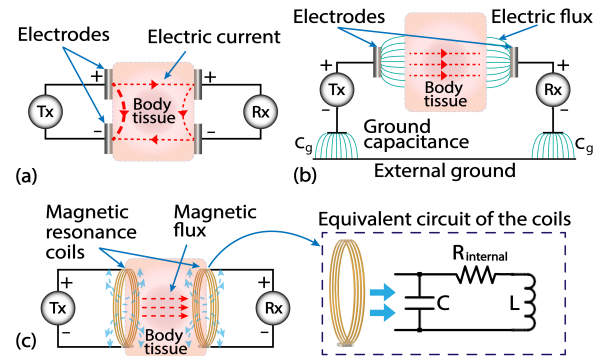


Fig. 1: Intra-body coupling methods: (a) galvanic coupling, (b) capacitive coupling, and (c) magnetic resonance coupling (MRC).

energy capacity (due to easily changed batteries), connection to external devices, and the possibility of supplying energy to other in-body nodes that cannot harvest enough energy on their own.

B. Human Body Communications and possible technologies

The communication ability (whether for information or energy transfer) is crucial for all such nodes. Although RF can be used by on-body nodes, RF does have some security issues, e.g., the possibility of eavesdropping, intrusion, or jamming by adversaries. Security vulnerabilities of IoT devices in general and in healthcare cases specifically as well, as noted in the recent report (<https://cps-vo.org/node/72664>), which states that 82% of healthcare organizations' IoT devices have been targeted with a cyberattack within the last year (compared with 80% of organizations overall) and only 7% of attacks had no financial impact. Through the body communications, popularly known as *Human Body Communications (HBC)*, can lessen this concern since the attacker would need to be in close proximity to the person to conduct an attack. Unfortunately, RF itself does not travel well through the body [5], and other mechanisms are needed.

Several HBC mechanisms have been explored in the literature. They require various forms of coupling of electrodes into the body such as galvanic coupling (GC) [6], capacitive coupling (CC) [7], and magnetic resonance coupling (MR) [8], [9]. Fig. 1 briefly illustrates their working principle.

Galvanic coupling (GC): The Galvanic HBC transmits the signal to the human body through a pair of electrodes that are placed in contact with the skin and act as a transmitter (T_x) and receiver (R_x) respectively. The two electrode pairs across

the body are shown in Fig. 1(a). Due to the low conductivity of the human body, the signal between the transmit and receive electrodes is rather small [10]. Most of the current flows locally because of the short spacing between the positive and negative terminals on each end. So, GC coupling is not an effective way to transfer energy or communicate across the body. To ensure the most effective communication, the GC signal frequency ranges from 10 kHz to 100 MHz. A recent study reported a data rate of 1.23 Mbps when transmitting at 200 kHz with attenuation levels typically around 50 dB over a distance of 15 cm [11].

Capacitive coupling: In capacitive coupling (also known as electrostatic coupling), electrodes T_x and R_x are used, as shown in Fig. 1(b). The ground electrodes are left floating while the signal electrodes are securely affixed to the body, creating a capacitance with the environment (ground or other objects around them). Capacitive coupling can be modeled using a distributed RC circuit [12]. Recent work shows an attenuation of 20–25 dB at 60 MHz and an on-body distance of 140 cm for capacitive coupling. Additionally, due to the weak nature of the received signal and high dependability on the surrounding environment, capacitive coupling in HBC usually works well only over a short-range [7] making it unusable for use with implantable or wearable devices at a longer distance.

Magnetic resonance coupling: Magnetic resonance coupling occurs when signals are coupled between the two coils T_x and R_x through magnetic flux as shown in Fig. 1(c). Both the transmitter and the receiver use an inductive coil in parallel with an identical capacitor to form a resonant LC circuit capable of transferring energy quite efficiently at resonance frequencies. Most MR coupling occurs over a spectral range between about 100kHz and 50 MHz, which produces a maximum attenuation of only 8.1 dB at a distance of 40 cm covered [11].

Ultrasonic coupling: Ultrasound coupling (USC) [13] is a very well-researched technology and has been widely used in various clinical applications [14], and specifically explored for both communications [15] and power transfer [16], [17]. USC is very popular for imaging in the human body, with typical frequencies in 3–6 MHz range. The USC velocity in human tissue varies in the range 1500–2000 m/s, which is quite slow but adequate for medical applications. However, this results in wavelengths of only 0.3–0.7 mm and has implications for penetration depth. Small USC devices have been used extensively in implants without any reported side effects, and provide a range of 5–10 cm communication range. USC can work quite well in on-body settings, particularly due to the phenomenon of Rayleigh surface acoustic waves (SAW) [18]. Surface acoustic waves travel along smooth surfaces and can cover significant distance without much attenuation; however, undulations in the surfaces of the order of a few wavelengths can disrupt them. For on-body applications, we have both scenarios, e.g., bare skin (typically quite smooth) and skin covered with clothing or other materials.

C. Our contributions

In this paper, we conduct a detailed experimental comparison of two promising technologies for on-body communication devices, i.e. MRC and USC. Our prior work on MRC has shown that it works better than other forms of HBC [19]–[21] and is very robust against variations that one would expect in on/in-body environment such as movement, posture, clothing, person to person variations (e.g., build, weight, etc.). It can also provide a range of almost the entire body-length with only about 25db loss. So, we believe that MRC is a good electronic communication mechanism for HBC use. On the other hand, ultrasound has also been explored extensively for intrabody use and therefore we chose this as a potential technology for HBC. We will experimentally explore the potential impact of SAW propagation on different surfaces.

Our experiments also seem to suggest that USC transmission works better with increasing frequency. This is again a likely result of the extremely complex environment inside the body. Overall, we find that USC works similar to or slightly better than MRC in 3–8 MHz.

D. Paper organization

The paper is organized as follows. In section II we discuss the magnetic and ultrasonic communication basics. Section III discusses our detailed experimental setup. The systematic comparison of magnetic and ultrasonic coupling through the human body is discussed in section IV. The paper is concluded in section V.

II. BACKGROUND ON RELEVANT COMMUNICATIONS TECHNOLOGIES

Because of their ubiquity, short-range RF based communication such as Bluetooth Low Energy (BLE) would be a natural choice for our application; unfortunately, RF is known to suffer high signal absorption in aqueous/tissue media [22]. We therefore discuss the brief characteristics of MRC and USC in this section, and study their performance on the human body in subsequent sections.

A. MRC Communication Characteristics

MRC works on the principle of magnetic induction between two coils, and the matching of resonance frequency on transmit and receive sides enhances the energy transfer between the two. MRC uses a LC-circuit as antenna on both transmit and receive side. Since a coil with inductance L and a capacitor with capacitance C has resonance frequency of $1/(2\pi LC)$, the resonant energy transfer is easy to achieve, and the antenna can be quite small. We considered a flat coil of diameter 20 mm that contacts the skin directly. The energy transfer in this case can be described by Lenz's law and the detailed equations are given in [23].




Fig. 2: The intersection angle between two unidirectional coils

Consider a transmit and receive coil pair separated by distance r with the plane of the coils tilted at angles β_t and β_r relative to the axis joining the coil centers, as shown in Fig. 2. Then the magnetic field induced in a receiver coil due to the current flowing through the transmit coil is given by Lenz's law. In particular, the mutual inductance in between the coils can be described as [24].

$$M_{t \rightarrow r} = M_{r \rightarrow t} \approx \frac{\mu \pi N_t N_r \rho_t^2 \rho_r^2}{2r^3} \left| \cos \beta_t \cos \beta_r - \frac{1}{2} \sin \beta_t \sin \beta_r \right| \quad (1)$$

Here ρ_x and N_x are the radius and the number of turns in the transmit ($x = t$) and receive ($x = r$) coils respectively, and μ is the magnetic permeability of the medium. In this paper, we assume that the transceivers are of identical dimensions, i.e. $N_t = N_r = N$ and $\rho_t = \rho_r = \rho$.

However, our experiments indicate that these equations do not accurately describe the signal propagation through the human body. The reason is that these equations are intended for simple media like air, but the human body environment is extremely complex. Overall, our earlier experimental work indicated that MRC works substantially better in human body than in the air [19], [21].

From the equation (1), it can also be seen that the induced magnetic field (and hence the induced current) in the receive coil is maximum when the planes of the two coils are aligned (i.e., $\beta_t = \beta_r = 0$), and goes down rapidly as the misorientation increases. However, our extensive experiments did not show much sensitivity to this misalignment [19]. From a practical perspective, this is highly desirable since the relative alignment will often be quite different and may change with body movement and posture change. As reported later in the paper, we find a similar issue even with USC for the human body.

B. USC Communication Characteristics

The working principle of ultrasound communication can be described as follows: the intensity I of USC waves (in mW/cm^2) can be related to the pressure P , the density of the media ρ , and the speed of sound c (1,540 m/s in tissue) as follows: $I = P^2/(\rho c)$. As the US wave propagates, the pressure at distance d , denoted $P(d)$ decreases from the initial pressure P_0 as $P(d) = P_0 e^{-\alpha d}$ where α (in nano-Pascal/cm) is the attenuation coefficient. It turns out that α is a function of the carrier frequency f as $\alpha = a f^b$ where a and b are attenuation parameters characterizing the media. With b close to 1 for body parts, α is approximately proportional to the frequency, which means that the attenuation in pressure at a given distance d should drop exponentially with f .

When vibration is applied to a free boundary, surface acoustic waves (SAWs) are always created and may be regarded as the superposition of two distinct components: longitudinal and transverse. SAWs can be categorized as Rayleigh waves that propagate across a solid-vacuum interface and form an interference pattern [18]. As the region of interest is the skin, those waves will decay quickly with distance. However, experimentally the communication range improves with frequency, at

least for the frequency range that we were able to experiment with (745 KHZ to 8 MHz). Since US waves are mechanical, they should scatter at boundaries between two materials (e.g., soft tissue and bone), according to Snell's law, which makes the overall intrabody behavior very complex.

III. EXPERIMENTAL EVALUATION OF MRC AND USC

A. Instruments used

Building out actual circuit boards for communication experiments is an extremely complex task; therefore, we have used available development platforms for this work. There are several such platforms [25], [26], and they typically utilize FPGAs or specialized CPU's for high-sample-rate digital signal processing. We chose USRP (Universal Software Radio Peripheral) [25] because of its widespread use and operating knowledge in the academia and industry. It consists of a motherboard and two daughterboards. The primary processing unit is the motherboard, which includes AD/DA converters (a dual 100 MSPS 14-bit ADC and a dual 400 MSPS 16-bit DAC) and an FPGA unit (Spartan 3A-DSP 3400). The daughterboards are radio frequency (RF) front ends that connect the device to a transmitter or receiving antennas. We utilize LFTX and LFRX daughterboards that run from DC to 30 MHz, which covers frequency range of interest that we are interested in.

We used USRP N210 and connected LFTX/LFRX to the antenna (USC or MRC) for our experiments. Such a setup allows us to transmit actual packets with suitable frame encoding. We used the simple BPSK (binary phase shift keying) in these experiments. It is certainly possible to use more sophisticated schemes (e.g., QPSK or higher) to increase the packet rate; however, high packet rate is usually not necessary in most healthcare/well-being applications; instead, the more important aspect is energy consumption, for which the simplest scheme is the best.

We measured both the packet received and power received at the receiver at different distances and frequencies. The transmit power was maintained at 0.3 mW throughout the study. It is reported under the safety threshold limit according to the IEEE standard for safety levels with respect to human exposure [27]. An unregulated exposure to non-static electromagnetic fields may adversely affect the health of humans [28]. There was no sensation reported throughout the duration of the experiment due to the low transmission power, which did not cause any localized heating or absorption by the tissue [19], [21]. Note that all distances were through-the-body distances, and each frequency change required a change of transmit/receive antennas and a re-calibration to ensure accurate measurements.

B. Experimental protocol with human subjects

All experiments in this study were conducted on the human body and in the air, the former being done under a fully approved by IRB protocol #28089 at Temple. The experiments here mostly involve a single middle-aged volunteer. Our earlier work [19] had conducted experiments on 6 very different adults and found the variations in received power among them confined to a few dB. Therefore, we believe that our

results are quite representative. Also note that since the many different points on the body were used for measurements, transmission path for both USC and MRC includes subcutaneous fat, muscles, bones, blood, etc. For practical reasons, all experiments had to be on-body; however, we have in the past done experiments by putting transmitter/receiver inside store-bought chickens. These results also indicate better transmission inside the body than in the air.

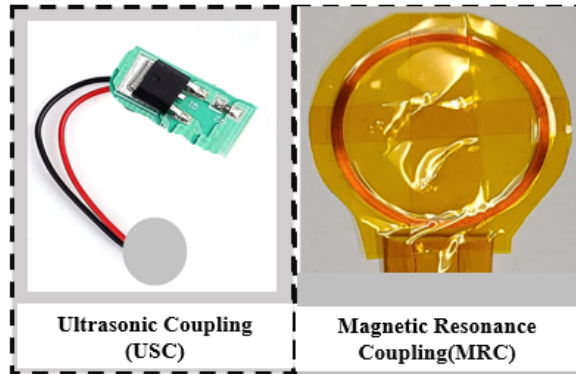


Fig. 3: Illustration of USC and MRC transceivers

Fig. 3 shows the pictures of USC and MRC transducers. USC transceivers were operated at 1, 3, 5, and 8 MHz frequencies. The USC transceivers were of disk form-factor with diameter of 20 mm, and thickness depending on the frequency; the thickness goes down with frequency, It is 2.1mm for 1 MHz, 0.7mm for 3 MHz and 0.4mm for 5 MHz. It is already too small (0.2mm) at 8 MHz, thereby requiring extreme care in attachment and issues of fragility. We were unable to easily order USC transceivers operating at even higher frequencies, although they can be custom ordered. Note that the USC output on the receiver side needs to be rectified to have a DC output. We built a standard full-rectifier bridge for this purpose.

The MRC experiments were also conducted at 3, 5, and 8 MHz. For MRC, the antenna consists of an LC circuit (coil and a capacitor). The coil diameter was again 20 mm, and the physical size of MRC and USC were similar. The inductance (made out of 7 turns of 34 AWG) of 7 μ H is used with the planar coil. The capacitance is 400pF for 3MHz, 140pf for 5 MHz and 56 pF for 8MHz. The transmitter and receiver coils were covered by a specialized magnetic shielding film (WMF200, Woremor) to minimize magnetic interference from nearby electronic equipment and over-the-air transmission [29]. The size is a crucial parameter for intra-body use, and a 20mm diameter is workable according to discussion with experts. The standard operating frequency for MRC is 13.56 MHz, but we tuned it down to lower frequencies by changing the capacitor and/or number of coil turns.

In a single run, 1000 packets were sent from the transmitter to the receiver for both USC and MRC. The distance between transmitter and receivers was incremented in steps of 3 cm, in 1-50 cm range. For both USC and MRC experiments, the transmitter was attached to the palm of the volunteer, and the receiver was placed on the ventral side of the arm and incrementally moved from the palm to the shoulder position. We ensured a good contact with the skin by using appropriate

gel (i.e., ultrasonic jelly for USC, and electrostatic jelly for MRC). Both transmitter and receiver transducers were taped over to keep them on securely. In the case of MRC, we used magnetic shielding of each to avoid through-the-air transmission but no such shielding is necessary for USC; however, we do need to mind the surface acoustic waves traveling along the skin surface between transmitter and receiver.

We used a simple packet structure to send packets, with a maximum length of 56B. The packet header consists of 2B preamble, 1B source/destination address, and a standard 2B CRC is added at the end to detect packet errors [21].

By a careful comparison between sent and received data, we found that in all cases, the CRC was able to detect the error; therefore, all packets received without the CRC error represent packets that do not suffer from any bit flips.

IV. RESULTS AND DISCUSSION

A. Comparison of USC with different frequencies

We first demonstrate the performance of our USC transceivers operating at different frequencies. The number of packets correctly received with varied transceiver distances is depicted in Fig. 4. We can see from this figure that the transmission range of USC-8MHz is $\sim$ 25 cm (with 100 percent packet delivery) and that this range decreases with the decrease in operating frequencies. Consequently, we may conclude that the USC performs better at higher frequencies; we hypothesize that this is due to ultrasound signals' complex propagation characteristics within the human body.

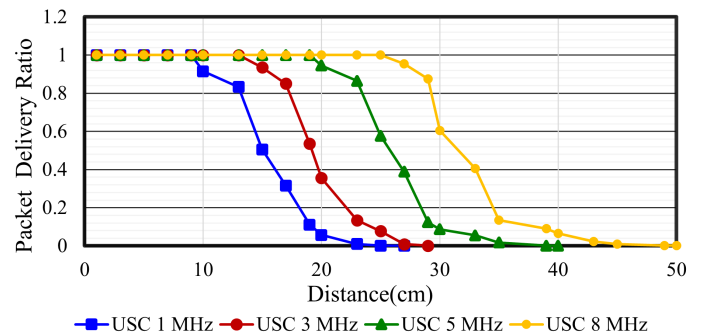


Fig. 4: Packet delivery ratio vs transceiver distances with different operating frequencies

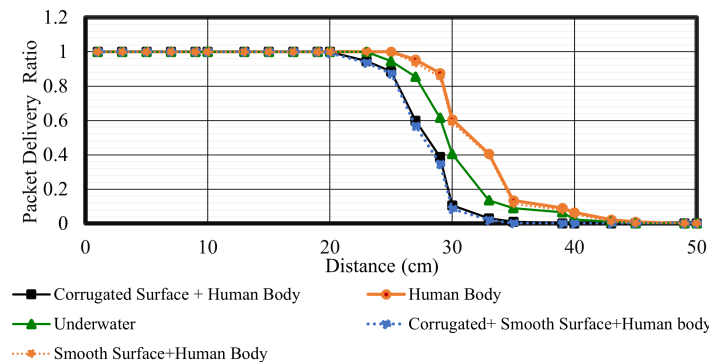


Fig. 5: Packet delivery ratio of USC with different surfaces at 8 MHz frequency

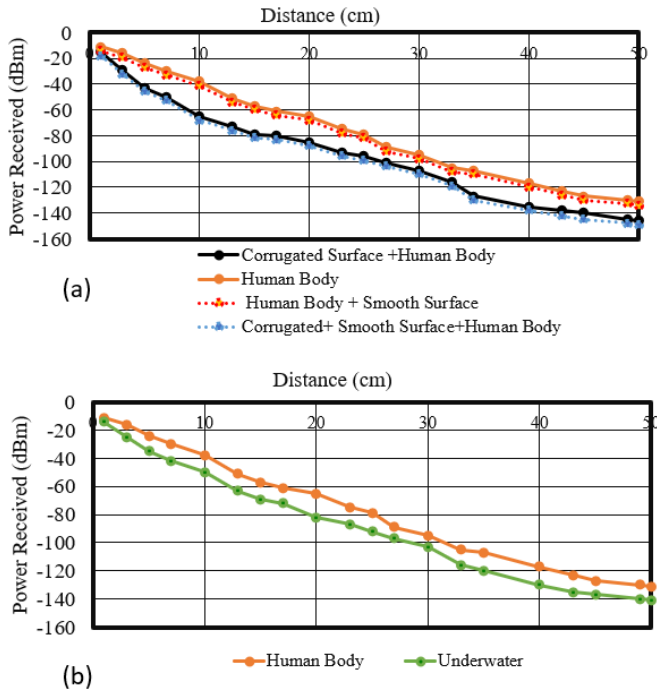


Fig. 6: Power received (dBm) of USC with different surfaces at 8 MHz frequency a) With different surface b) With underwater versus human body

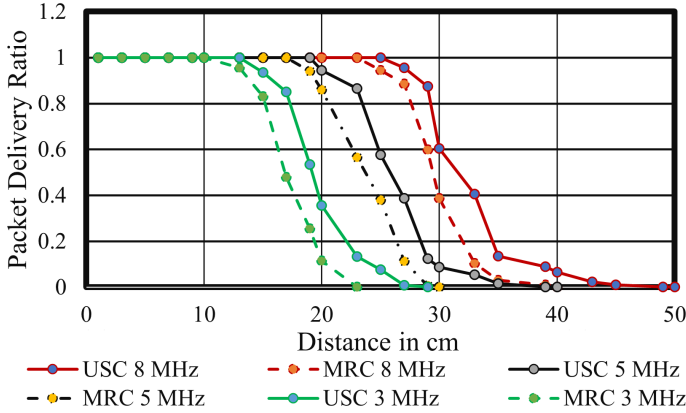


Fig. 7: Packet delivery ratio vs distances in USC and MRC

B. Ultrasonic communication with different surfaces

Due to the phenomena of Rayleigh surface acoustic waves (SAW), USC works well on the body. However, surface acoustic wave (SAW) is an acoustic wave traveling along the surface of a material exhibiting elasticity, with an amplitude that typically decays exponentially with depth into the material, such that they are confined to a depth of about one wavelength.

We now illustrate the influence of smooth, corrugated, and underwater surfaces on USC. The results are depicted in Fig. 5 and 6, respectively. The following two scenarios were devised to demonstrate the effects on smooth surfaces: (a) cover the transceivers with cloth, and (b) cover the medium (in this example, the arm) in between the transceivers with a cloth. In order to conduct these experiments, we utilize a cotton fabric with a thickness of ~ 5 mm. We can see from Fig. 5 that the influence of clothing is almost non-existent, which

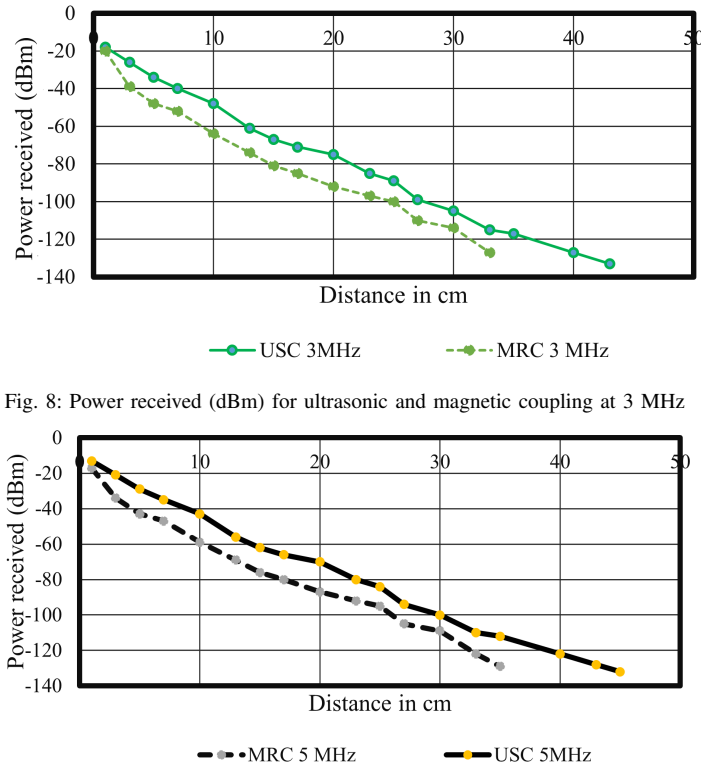


Fig. 8: Power received (dBm) for ultrasonic and magnetic coupling at 3 MHz

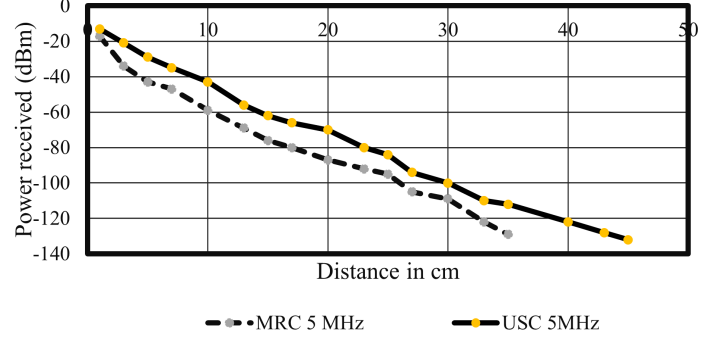


Fig. 9: Power received (dBm) for ultrasonic and magnetic coupling at 5 MHz

makes it appropriate for scenarios in which the wearables are worn within everyday clothes. The body environment is largely water and we have done underwater tests to check if the results would be consistent with intrabody propagation. To observe the propagation properties, we fill a few boxes with tap water and observe that this improves the transmission range to ~ 47 cm for underwater as shown in Fig. 6 (b). The high water content of the human body is also a contributing factor; the transmission range is nearly the same as that found underwater.

We then repeated the experiment using corrugated cardboard to cover the arm instead of clothing. To provide a fair comparison with the garment impacts, we maintain the corrugated surface thickness at ~ 5 mm. As seen in Fig. 6(a), the corrugated surface significantly dampens the signal, resulting in decreased packet delivery, as illustrated in Fig. 5. We hypothesize that the difference in effects between corrugated and clothes is mainly related to the porosity of clothing materials compared to solid corrugated cardboard, although more research is necessary to validate this. In summary, the corrugated surface significantly affects the surface acoustic wave but does not affect the garment materials.

C. Ultrasonic vs Magnetic Resonance coupling

Our experiments indicate that both MRC (see [18]) and USC show favorable propagation characteristics on the human body; therefore, we compare these two technologies' effects in this section. The transceiver details are reported in subsection III-B. This comparative study is shown in Figs. 7-10, where we varied the operating frequencies from 3-8 MHz. This comparative study indicates that both USC and MRC show very similar

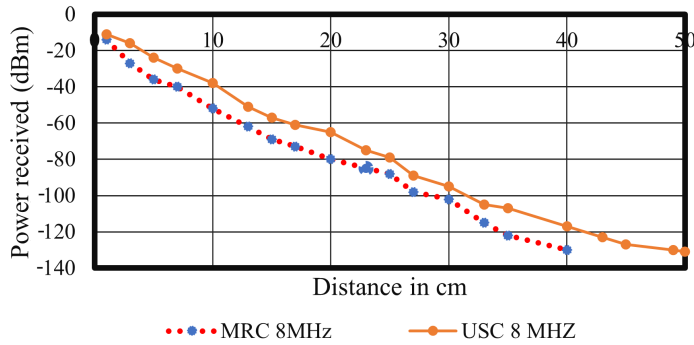


Fig. 10: Power received (dBm) for ultrasonic and magnetic coupling at 8 MHz

relative behavior in 3-8 MHz. USC performs marginally better than MRC in this band. For example, at 8 MHz, the packet delivery drops to $\sim 80\%$ at 30 cm for USC; with the same delivery performance, the range drops to ~ 28 cm for MRC. A higher water concentration in the body might be helping ultrasonic waves achieve a more extended range. However, further experimentation with other frequency bands needs to be conducted to strengthen this claim further.

V. CONCLUSIONS AND FUTURE WORK

In this paper, we have compared ultrasonic coupling versus magnetic resonance coupling-based communication for application in on-body and intra-body nodes (with the signal being communicated within the body). We showed that ultrasonic coupling (USC) works much better than magnetic resonance coupling (MRC) for transmission through the body at 8 MHz frequency. Specifically, it is seen that at 0.3 mW transmitted power, USC based communication shows a range of 50 cm without data loss, whereas MRC shows comparable performance only up to 40 cm (25% increase in communication range for USC based communication). Future work will involve exploration into frequencies above 8 MHz. This was not done in the current study since higher frequency USC transducers need to be custom ordered and are not easy to procure. They would also be much thinner, thus making their use challenging. We will also examine the robustness of ultrasound communications under various scenarios and with different volunteers similar to what we have already done with MRC.

ACKNOWLEDGEMENTS

The project was supported by the National Science Foundation (NSF) grants ECCS-2029077 (PI A. Kim), and CNS-1844944 (PI K. Kant). The authors would also like to acknowledge Prof. Albert Kim and graduate student Sayemul Islam from Temple University (Philadelphia, PA, USA) for their help with the experiments.

REFERENCES

- [1] S. Seneviratne *et al.*, "A survey of wearable devices and challenges," *IEEE Communications Surveys & Tutorials*, vol. 19, pp. 2573–2620, 2017.
- [2] L. P. Fried, "America's health and health care depend on preventing chronic disease," https://www.huffingtonpost.com/entry/americas-health-and-healthcare-depends-on-preventing_us_58c0649de4b070e55af9eade, March 2017.
- [3] A. Mendez *et al.*, "Estimation of bladder volume from afferent neural activity," *IEEE Transactions on Neural Systems and Rehabilitation Engineering*, vol. 21, pp. 704–715, 2013.
- [4] K. Kaszala *et al.*, "Device sensing: sensors and algorithms for pacemakers and implantable cardioverter defibrillators," *Circulation*, vol. 122, pp. 1328–1340, 2010.
- [5] D. Werber *et al.*, "Investigation of RF transmission properties of human tissues," *Advances in Radio Science*, vol. 4, pp. 357–360, sep 2006.
- [6] W. J. Tomlinson *et al.*, "Galvanic coupling intra-body communication link for real-time channel assessment," in *IEEE INFOCOM Workshops*, 2016.
- [7] A. Datta *et al.*, "Advanced biophysical model to capture channel variability for eqs capacitive hbc," *bioRxiv*, 2020.
- [8] Y. K. Hernandez-Gomez *et al.*, "Magnetic human body communication based on double-inductor coupling," in *IEEE I2MTC*, 2017, pp. 1–6.
- [9] S. Banou *et al.*, "MAGIC: Magnetic Resonant Coupling for Intra-body Communication," in *IEEE INFOCOM*, 2020, pp. 1549–1558.
- [10] B. Kibret *et al.*, "Investigation of galvanic-coupled intrabody communication using the human body circuit model," *IEEE Journal of Biomedical and Health Informatics*, vol. 18, pp. 1196–1206, 2014.
- [11] J. Park *et al.*, "Magnetic human body communication," in *IEEE EMBC*, 2015, pp. 1841–1844.
- [12] N. Cho *et al.*, "The human body characteristics as a signal transmission medium for intrabody communication," *IEEE Transactions on Microwave Theory and Techniques*, vol. 55, pp. 1080–1086, 2007.
- [13] R. Cavallari *et al.*, "A survey on wireless body area networks: Technologies and design challenges," *IEEE Communications Surveys Tutorials*, vol. 16, pp. 1635–1657, Third 2014.
- [14] B. Sigel, "A brief history of doppler ultrasound in the diagnosis of peripheral vascular disease," *Ultrasound in medicine & biology*, vol. 24, pp. 169–176, 1998.
- [15] L. Galluccio *et al.*, "Challenges and implications of using ultrasonic communications in intra-body area networks," in *2012 9th Annual Conference on Wireless On-Demand Network Systems and Services (WONS)*. IEEE, 2012, pp. 182–189.
- [16] A. Ibrahim *et al.*, "A comprehensive comparative study on inductive and ultrasonic wireless power transmission to biomedical implants," *IEEE sensors journal*, vol. 18, pp. 3813–3826, 2018.
- [17] K. Agarwal *et al.*, "Wireless power transfer strategies for implantable bioelectronics," *IEEE Reviews in Biomedical Engineering*, vol. 10, pp. 136–161, 2017.
- [18] A. C. Saavedra *et al.*, "Measurement of surface acoustic waves in high-frequency ultrasound: Preliminary results," in *2017 39th Annual International Conference of the IEEE Engineering in Medicine and Biology Society (EMBC)*, 2017, pp. 3000–3003.
- [19] S. Islam *et al.*, "Performance evaluation of magnetic resonance coupling method for intra-body network (ibnet)," *In process for IEEE Transactions on Biomedical Engineering*, Oct 2021.
- [20] R. Gulati *et al.*, "Experimental evaluation of a near-field magnetic induction based communication system," *IEEE WCNC*, 2019.
- [21] R. K. Gulati *et al.*, "Characterization of magnetic communication through human body," *IEEE CCNC*, 2022.
- [22] R. Jedermann *et al.*, "Communication techniques and challenges for wireless food quality monitoring," *Philosophical Transactions of the Royal Society*, vol. 372, p. 20130304, 2014.
- [23] A. Pal *et al.*, "Nfmi: Near field magnetic induction based communication," *Elsevier Computer Networks*, Nov 2020.
- [24] X. Tan *et al.*, "Environment-aware indoor localization using magnetic induction," in *IEEE GLOBECOM*, 2015, pp. 1–6.
- [25] U. S. R. Peripheral, "Universal software radio peripheral," <http://www.ettus.com/>, accessed: Aug 2021.
- [26] R. University, "Warp: Wireless open-access research platform," <http://warpproject.org>, accessed: Aug 2021.
- [27] "IEEE standard for safety levels with respect to human exposure to electric, magnetic, and electromagnetic fields, 0 hz to 300 GHz," 2019. [Online]. Available: <https://doi.org/10.1109/ieeestd.2019.8859679>
- [28] "Guidelines for limiting exposure to time-varying electric and magnetic fields (1 Hz TO 100 kHz)," International Commission on Non-Ionizing Radiation Protection, Tech. Rep. 6, 2010.
- [29] M. Bailleul, "Shielding of the electromagnetic field of a coplanar waveguide by a metal film: Implications for broadband ferromagnetic resonance measurements," *Applied Physics Letters*, vol. 103, p. 192405, Nov. 2013. [Online]. Available: <https://doi.org/10.1063/1.4829367>