Hyperspectral Dark Field Optical Microscopy for Orientational Imaging of a

Single Plasmonic Nanocube using Physics-based Learning Method

Nishir Mehta<sup>1</sup>, Amirreza Mahigir<sup>2,3</sup>, Georgios Veronis<sup>2,3</sup>, Manas Ranjan Gartia<sup>1,\*</sup>

<sup>1</sup>Department of Mechanical and Industrial Engineering, <sup>2</sup>School of Electrical Engineering and

Computer Science, Louisiana State University, Baton Rouge, Louisiana 70803, USA

<sup>3</sup>Center for Computation and Technology, Louisiana State University, Baton Rouge, Louisiana

70803, USA

\*E-mail: mgartia@lsu.edu

**Abstract** 

Rotational dynamics at the molecular level could provide additional data regarding protein

diffusion and cytoskeleton formation in cellular level. Due to the isotropic emission pattern of

fluorescence molecules, it is challenging to extract rotational information from them during

imaging. Metal nanoparticles show polarization-dependent response and could be used for sensing

rotational motion. Nanoparticles as an orientation sensing probe offer bio-compatibility and

robustness against photo-blinking and photo-bleaching compared to conventional fluorescence

molecules. Previously, asymmetric geometrical structures such as nanorods have been used for

orientational imaging. Here, we show orientational imaging of symmetric geometrical structures

such as 100 nm isolated silver nanocubes by coupling a hyperspectral detector and a focused ion

beam (FIB)-fabricated correlating substrate. More than 100 nanocubes are analyzed to confirm

spectral shifts in the scattering spectra due to variations in the orientation of the nanocubes with

respect to the incoming light. Results are further validated using finite-difference time-domain

1

simulations. Our observations suggest a novel strategy for high-throughput orientation imaging of nanoparticles.

## 1. Introduction

Orientation of nanostructures is critical in many applications such as the detection of single polymer chains in biomedicine [1, 2], catalysts [3], DNA biosensors [4], protein interactions and detection [5], hotspots of surface-enhanced Raman spectroscopy (SERS) [6], opto-magnetic data storing devices [7], and fluorescence resonant energy transfer (FRET) [8, 9] experiments. Control over orientation is vital in order to modify single nanoparticles to create Janus particles, as well as to create dimers by placing two different metal nanostructures in close vicinity [10, 11]. Understanding the interactions of nanoparticles of different shapes and orientations with cell membranes is crucial in drug transport and gene delivery [12-15]. Younan Xia's group [16] compared the intake of gold nanocubes, nanorods and nanohexapods for photothermal cancer treatment, and found that nanohexapods have better internalization than nanocubes and nanorods. Hu et al. [17] found that vertical orientation of ellipsoid nanoparticles is more effective for phagocytosis compared to horizontal orientation. This is because of the better alignment of the vertical orientation during macrophage phagocytosis [18, 19]. The roles of shape, aspect ratio, and orientation on the cellular internalization process were previously demonstrated experimentally and using molecular dynamics simulations [20-23]. However, it is difficult to acquire the actual orientation of a nanostructure using standard optical microscopes due to the optical diffraction limit.

Conventional techniques to characterize nanoparticles, such as fluorescence imaging [24, 25] and magnetic resonance spectroscopy [26] involve complex sample preparation, probing, and labeling

expertise. Existing methods of interrogation of nanoparticles like fluorescence polarization spectroscopy are not suitable for studying single-particle ensembles, are time intensive, expensive, and require many resources for sample preparation and analysis. At the same time, conventional optical microscopes are limited by diffraction (to approximately 250 nm) [27] and only provide intensity images without spectral information. Due to inhomogeneous and uncontrolled labeling, there is a loss of information and generation of artifacts that offer false impressions generating erroneous data [28]. Previously, absorption-based photothermal imaging [29], single- and two-photon luminescence [30], and defocused imaging [31] methods were used to study the orientation of a single nanoparticle. In previous studies, a laser was utilized, and wherein laser generates heat which creates possibilities of thermal deformation [32] and limits applications in biology/soft matters. A challenge in defocusing microscopy [33] is its inability to accurately determine the spectral distribution without reducing the quality of the image.

Polarized-scattered-light-based plasmonic orientation sensing has been performed by the direct fitting of the cosine squared function to angular intensity profiles [34] and by using polarization-dependent color change, where images were collected at only a few spectral bands [35]. Kim et al. [36] performed a comprehensive study in which polarization-dependent color change of low aspect ratio (AR=1.5) gold nanorods (AuNRs), non-optimal color assignments, and near-infrared plasmon resonances were studied. However, information was limited to three color channels (and the CCD detector) – three data points and orientation assignments based on the underlying colorimetric change.

Polarized dark-field hyperspectral microscopy provided a five-fold improvement in determining the orientation of the nanoparticles compared to photothermal and defocused imaging [37]. The use of a broadband light source allowed to achieve wide-field and hyperspectral imaging capabilities compared to photothermal imaging. High-throughput high-accuracy orientational studies of nanostructures via polarized scattering microscopy require a novel protocol. The polarization of the incoming light affects the plasmonic resonances. Light scattered or absorbed by the nanoparticles can be quantified to reflect orientation as well as other intrinsic properties. Previously studies have used AuNRs, which have one less axis of symmetry than nanocubes. Recently, Teri Odom's group [38] described a machine learning method for nanorods and nanostars to determine the orientation using differential interference contrast (DIC) images.

In this paper, we evaluate cubical (more complex) probes and report different intensity peaks for diagonal and planar oscillation modes compared to longitudinal and transverse modes in nanorods. We also demonstrate spectral information in more than three bands (hyperspectral) in the visible and near-infrared (VNIR) wavelength range. Super-imposition of spectroscopic data over the CCD-imaged data allows us to quantify orientation changes based on spectral shift, in contrast to qualitative color change demonstrated in previous studies. We perform correlative studies between quantified spectral features and scanning electron microscopy images. Unlike previous studies, we perform finite-difference time-domain (FDTD) numerical simulations to confirm the experimental results. Our results demonstrate a new platform application for orientational imaging with single nanoparticle resolution.

#### 2. Materials and Methods

**Materials:** ITO slides were purchased from Sigma Aldrich. Polyvinylpyrrolidone (PVP) silver nanocubes were purchased from nanoComposix, Inc.

**Structural characterization:** High-resolution transmission electron microscopy (TEM) images of the nanocubes were acquired with JEOL JEM-2011 equipped with a Gatan SC1000 CCD camera.

Sample preparation: We drop-cast the 100-nm Ag nanoparticles on a 75 mm ITO-coated glass slide. Prior to drop-casting, we etch the patterns in the ITO-coated slides via focused-ion beam milling. A focused gallium ion beam tilted at 52 degrees allows for nano and micro-scaled cutting of substrate in order to index individual nanoparticles. Square arrays of X-Y dimensions 1-1.5  $\mu$ m were generated for a fine view of 100 nm nanocubes. The micro-milled glass substrate is preheated in an oven to 40 degrees for 10 minutes before drop-casting particles to prevent coffee-ring phenomena in nanostructure distribution by quickly eliminating the water solution. Next, a 5  $\mu$ L solution containing silver nanocubes was drop-coated on an indexed glass slide, and water was allowed to vaporize. An electron beam analytical tool such as scanning electron microscopy (SEM) is used to determine the angular orientation of the nanostructure with respect to the indexed substrate. SEM images are processed in ImageJ software to provide angular assignment of individual nanostructures. A UV-6300 double beam spectrophotometer is used to investigate the wavelength range for plasmon resonance due to scattering from nanostructures in solution.

Hyperspectral imaging: A CytoViva hyperspectral microscope equipped with a high-intensity halogen light source was used to provide hyperspectral imaging in the wavelength ranges of  $\lambda = 400\text{-}1000\,\text{nm}$ . A liquid light guide was used to focus light at oblique angles through the illumination condenser. The spectral resolution obtained is 2 nm, and the spatial area of each pixel is 25 nm x 25 nm. An oil objective with 100x magnification was used to acquire the images. Immersion oil contributes to reducing the speed of light, thereby shortening the wavelength while at the same time keeping the frequency constant, according to the relation  $\lambda = \frac{2\pi c}{\omega}$  Where c is the

speed of light and  $\omega$  is the angular frequency [39]. To minimize random glare, we used a polarizing filter between the condenser and the glass substrate. Particles were sandwiched by gently placing a coverslip over the substrate. The coverslip was sealed using nail polish to avoid oil moving into the sample space. The exposure time for each pixel was 0.25 sec. We used the hyperspectral spectrograph to collect spectral data at room temperature. To improve signal-to-noise ratio, the intensity count was adjusted between 1000 and 10000. The image analysis was performed using the ENVI 4.8 software (CytoViva®, Inc.) in dark-field mode. Spectral data of nanoparticles obtained from experiments and simulations were normalized to a maximum intensity of 1. After carefully subtracting background irregularities, regions of interest were defined to collect spectra from selected pixels containing nanostructures. No special tagging or staining was done for the nanostructures. PCA data analysis and spectrum plotting were performed using the OriginLab software.

Computational method: FDTD simulations were performed using Lumerical FDTD Solutions. The refractive index of silver was obtained from CRC data [40], and the refractive index of glass used was 1.51. The mesh size was chosen equal to 2 nm throughout the simulation domain, which was terminated to perfectly matched layers (PMLs) in all directions. We used the total-field scattered-field formulation with a plane wave normally incident from the top as the pump signal to excite the nanostructure from  $\lambda = 400 - 900$  nm. The local electric field distribution in the surface of the nanocube at the resonance frequency was obtained using a plane frequency-domain field monitor.

**Orientation detection algorithm:** We constructed a large dataset of scattering spectra of nanocubes observed with hyperspectral microscopy and FDTD simulations. We then labeled the orientation of the nanocube in each spectra by comparing them with the FDTD simulations and

validated our algorithm using a correlative imaging approach (SEM images). We trained the model to interpret the spectra. Using what it "learned" from that dataset created by "physics-based" electromagnetic FDTD simulations, the resulting model can use new scattering spectra (obtained with a hyperspectral microscope) to predict the orientation of a nanoparticle (in this case of a nanocube). The similarity between the unknown spectrum and the library spectrum is identified by the spectral correlation coefficient (SCC) calculated using the following equation:

$$SCC = \frac{(Library \cdot Unknown)^2}{(Library \cdot Library)(Unknown \cdot Unknown)},$$

where *Unknown* denotes the spectrum of the nanocube for which orientation is sought, and *Library* denotes the reference spectrum in the constructed library. The *SCC* approaches 1.0 when the library spectrum and the unknown spectrum are similar. The SCC will approach 0, when there is no similarity between the library spectrum and the unknown spectrum.

## 3. Results and Discussion

The optical properties of metal nanoparticles are significantly dominated by surface plasmons associated with electron oscillations. Photon energies in the visible and mid-infrared regions of the light spectrum are sufficient to excite the surface plasmons of nanostructures [39]. The plasmon resonance characteristics of the nanoparticles depend mainly on the particle size, shape and orientation, especially when the structures are small compared to the incident light wavelength [41]. The optical response due to surface plasmons is dominated by the orientation of the nanostructures when probing structures with similar size and shape. Figure 1a shows schematically the physics-based learning method that we use to determine the orientation of a plasmonic nanoparticle. To challenge the algorithm, we select a highly symmetric nanoparticle, i.e. a silver

nanocube with 100 nm in length dimensions. Figures 1b and 1c show representative TEM images of a single nanocube. From the image analysis (Figure 1f) of several nanocubes, the average edge length of the nanocubes was found to be ~100 nm. Figure 1d shows the corresponding dark field image of the nanocubes. Figure 1e shows the experimental extinction coefficient spectra of ensemble nanocube particles in solution (water). The experimental extinction spectra exhibit several peaks. The peaks at  $\lambda = 347$  and 393 nm are due to the bulk plasmon resonance of Ag. Nanocubes in water showed two other intense peaks at  $\lambda = 466$  and 547 nm. The origin of these peaks was identified by performing FDTD simulations of nanocubes in water (Figure 1h). The locations of these extinction maxima are found to be size-dependent (Figures S1a and S1b). Increase in the edge length of the cube leads to a red shift in the absorption maxima due to the retardation effect (Figure S1c). The FWHM of the absorption peaks increase with the increase in the cube edge length and the peaks become less intense (Figures S1a, S1c). By comparing the contribution of scattering and absorption to the extinction spectra, we found that scattering plays a bigger role compared to absorption (Figure S1d). The theoretical spectra of the nanocubes are shown in Figure 1g. The plasmon modes of the nanocubes are also dependent on the corner geometry, i.e. the sharpness of the nanocube corner. Figure 1g compares the absorption spectra of single nanocubes with either sharp or rounded corners. The peak plasmon resonance of the rounded- cornered nanocube ( $\lambda_{peak} = 494$  nm, FWHM = 56 nm) showed a blueshift in the resonance wavelength compared to the sharp-cornered nanocube ( $\lambda_{peak} = 520$  nm, FWHM = 43 nm). The corner geometry has a strong influence on the plasmon resonance because of the dependence of the charge density distribution on the corner geometry. The distributions of electric field intensity  $(|E|^2)$  and charge density are shown in Figures 1h and 1i, respectively. The dominant mode (peak 1) has its induced charges concentrated at the cube's corner, and the positive and negative charges

are situated on each side. Thus, they have a large dipole moment p = qd, where q is the charge, and d is the cube's edge length, and hence couple strongly to light. Further, peak 1 corresponds to a dipolar mode, whereas peaks 2-4 correspond to multipolar modes.

Figure 2 shows the FDTD simulated scattering spectra of a nanocube in the air at different orientations with respect to the polarization direction of the incoming illumination. We see redshifts in the scattering peaks for the nanocubes that are oriented at 22.5°, 45°, and 67.5° compared to the nanocube at 0°. The corresponding electric field distributions are shown in Figures 2b – 2g. Comparison of the charge density distribution of a nanocube in air vs a nanocube on ITO showed that their dominant modes are different [42]. The dominant mode for a nanocube in air is dipolar (D), whereas for a nanocube on ITO slides it is primarily quadrupolar (Q) (Figures 2h – 2k). The dipole moment of a nanocube in air is much larger compared to the dipole moment of a nanocube on ITO (Figures 2j - 2k). Hence, it is difficult to couple the quadrupolar mode to the incident light. The magnitude of induced charge is dependent on the dielectric constant of the substrate as  $\frac{\varepsilon_s - 1}{\varepsilon_s + 1}$ ;  $\varepsilon_s = 1.0$  for air,  $\varepsilon_s = 1.77$  for water, and  $\varepsilon_s = 3.46$  for ITO. In air, the D and Q modes do not interact. On ITO, the D and Q modes interact forming hybridized bonding and antibonding modes. The antibonding mode (D-Q) has higher energy (shorter wavelength) compared to the bonding mode (D+Q) (as bond formation requires some energy). The antibonding mode (D-Q) loses energy with  $\theta$ , but does not shift its peak position, whereas the bonding mode (D+Q) shifts its peak position with  $\theta$  (Figure 2a). The shift between the positions of bonding and antibonding modes  $(\lambda_{D+Q} - \lambda_{D-Q})$  for ITO (= 160 nm) is much larger than the one for air (= 85 nm). The peak position of the bonding mode redshifts with the increase of the dielectric constant (  $\lambda_{D+Q}$ = 488 nm for air, 600 nm for water, and 619 nm for ITO) (Figure 21). The corresponding FWHM linewidths are 100 nm, 289 nm, and 140 nm for air, water, and ITO, respectively (Figure 21).

To determine the angle of a single nanoparticle, we use correlative microscopy to obtain scanning electron microscopy and dark-field optical microscopy data from the same sets of nanoparticles. Correlation was achieved by generating distinctive marker grids on the light-transparent ITOcoated glass slides [43]. Focused ion beam (FIB) milling was used to generate sharp 90° angled grooves of ~0.5 µm depth using high ion beam energy of 20 keV (Figure 3a). The dark field optical image and the corresponding hyperspectral image are shown in Figures 3b and 3c, respectively. The SEM image presented for the selected area (Figure 3a) clearly shows the nanocubes. The orientation is determined with respect to the square groove horizontal lines. The scattering spectra of the nanocubes (#P1 – P16) collected by the hyperspectral detector are shown in Figure 3e. The angular orientations of the particles are analyzed by the ImageJ software. Comparison of the linewidth of the pixels across a single nanoparticle as captured in SEM (FWHM ~ 100 nm) and of the same nanoparticle as it appears in a diffraction-limited hyperspectral dataset image (FWHM ~500 nm) is shown in Figure 3d. For transforming the high dimensional spectral data into a data set with reduced dimension, we used an unsupervised statistical technique, the principal component analysis (PCA) [44, 45]. We have previously used PCA approach for Raman spectral analysis [46, 47]. PCA result (Figure 3f) showed that the first principal component (PC1) can distinguish between single nanoparticles (+PC1 values) and multiple particles (-PC1 values) in a hyperspectral image. We found that PCA has an angular accuracy of  $\sim 45^{\circ}$  (Figure 3g).

Figure 4a shows an example of two nanocubes with different orientation, their corresponding hyperspectral images, and their scattering spectra. It shows the spectral distribution of the scattered light from a single nanocube particle. We have analyzed more than 100 nanocubes (see Figure

S2). We observe that the peak values lie between 652-657 nm when the orientation of the nanocubes is ~67.5° or 22.5°, whereas the peak values lie between 630-635 nm when the orientation of the nanocubes is  $\sim 0^{\circ}$  or 45°. We observe redshifts of  $\sim 12-15$  nm in the peak of the spectra for particles that are oriented with  $15^{\circ} < \theta < 35^{\circ}$  and  $60^{\circ} < \theta < 80^{\circ}$  with respect to the spectrum obtained at  $\theta = 0^{\circ}$ . We observe that particles with orientation  $\theta$  and  $(90^{\circ} - \theta)$  show similar scattering spectra. The FDTD simulation results (Figures 4c-4d) match with the experimental spectra shown in Figure 4b. Finally, we correlate the angles obtained from the SEM images for 44 nanocubes with the scattering spectra obtained using the hyperspectral microscope (Figure 4e). The predicted angle for the scattering peak using FDTD is plotted against the experimental angle in Figure 4f. The results showed Pearson's correlation r = 0.86, indicating good correlation [48] between the experimental and predicted results. The Pearson correlation coefficient (PCC) [49, 50] measures the extent of linear correlation between two data sets. The close correspondence between FDTD simulation and experimental results indicates that a hyperspectral system coupled with simulated spectra libraries could be used for quick, label-free and cost-efficient analysis of nanostructures.

# 4. Conclusions

In this study, we developed the optical imaging correspondence between hyperspectral data and scanning electron microscopy using a patterned substrate. Validation of the experimentally obtained results with FDTD numerical simulations and electron microscopy techniques allowed us to confirm the validity of our nanocube orientation assignments. We exploited the capability to probe the orientational dependence of the extinction cross section of a single nanocube. High-throughput imaging has been performed and the corresponding orientation of the nanocubes has been identified using the developed method. Furthermore, reference spectral libraries can be built

and stored in order to develop a protocol for precise and high-throughput machine learning-driven

analysis to determine the orientation of scattering nanoprobes.

**Author Information** 

Corresponding author

\* Manas Ranjan Gartia, Telephone: +1-225-578-5900

E-mail: mgartia@lsu.edu

**Author contributions** 

Nishir Mehta: Data curation; Formal analysis; Investigation; Software; Writing – Original Draft

Preparation (lead). Amirreza Mahigir: Investigation; Software. Georgios Veronis:

Conceptualization (supporting); Resources; Supervision; Writing – Review & Editing. Manas

Ranjan Gartia: Conceptualization (lead); Funding Acquisition; Methodology; Project

Administration; Resources; Supervision; Writing – Original Draft Preparation (supporting);

Writing – Review & Editing.

**Conflict of Interest** 

There are no conflicts to declare.


Acknowledgments

M.R.G. acknowledge the support from National Science Foundation (NSF CAREER award

number: 2045640). Scanning Electron Microscopy (SEM) and Transmission Electron Microscopy

(TEM) were performed at the Shared Instrumentation Facility (SIF) at Louisiana State University.

12

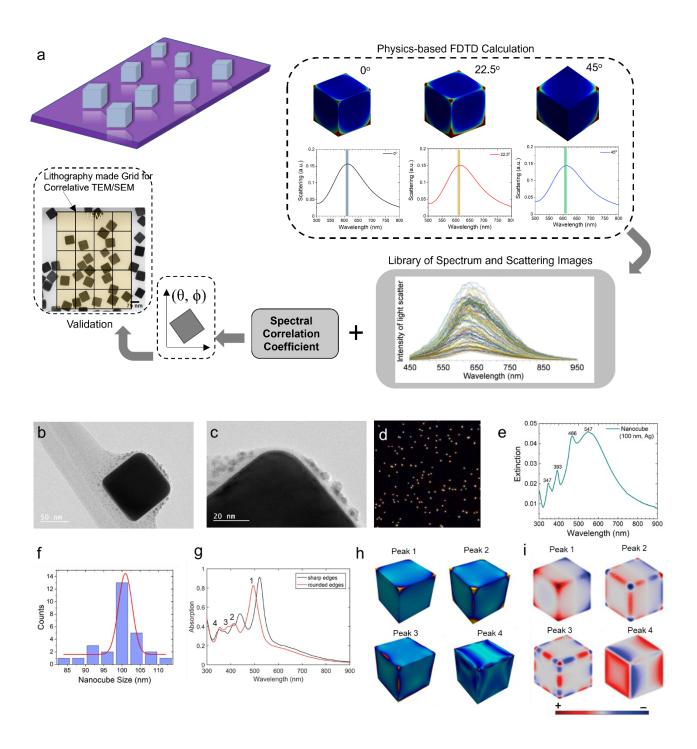

**Figure 1. (a)** Schematic of Ag nanocubes isolated and drop-casted on the substrate; Schematic of the physics-based learning method that we use to determine the orientation of a plasmonic nanoparticle; **(b-c)** Transmission electron microscopy (TEM) images of a single nanocube; **(d)** 

Dark-field image of nanoparticles taken using an optical image detector; (e) Extinction spectra of the nanocube sample collected in VNIR (visible-near infrared range) using a UV-Vis spectrophotometer; (f) Size distribution of nanocubes obtained from the TEM images using ImageJ. The average nanocube edge length is 98.5 (g) Absorption spectra of a nanocube in water using finite-difference time-domain (FDTD) simulations. Results are shown for nanocubes with sharp edge (black curve) and round edge (red curve); (h) The distribution of electric field intensity  $(|E|^2)$ , and (i) the corresponding charge density distribution on the nanocube.

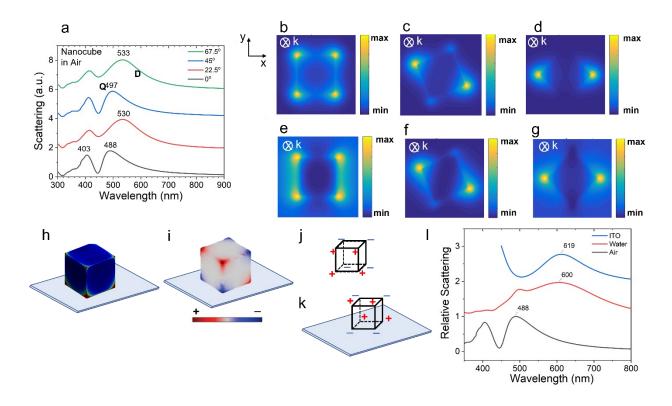


Figure 2. (a) Scattering spectra of a nanocube in air at different orientations calculated using FDTD. The dipole (D) and quadrupole (Q) modes are marked in the plot; Electric field intensity distribution at (b)  $\lambda = 404$  nm,  $\theta = 0^{\circ}$ ; (c)  $\lambda = 414$  nm,  $\theta = 22.5^{\circ}$ ; (d)  $\lambda = 412$  nm,  $\theta = 45^{\circ}$ ; (e)  $\lambda = 486$  nm,  $\theta = 0^{\circ}$ ; (f)  $\lambda = 533$  nm,  $\theta = 22.5^{\circ}$ ; and (g)  $\lambda = 497$  nm,  $\theta = 45^{\circ}$ ; Distribution of (h) electric field intensity, and (i) charge density of a nanocube on ITO substrate. The schematics of the corresponding charge distributions are shown for nanocubes (j) in air, and (k) on ITO substrate; (l) Normalized scattering spectra of a nanocube in air, water, and on ITO substrate obtained using FDTD simulations.

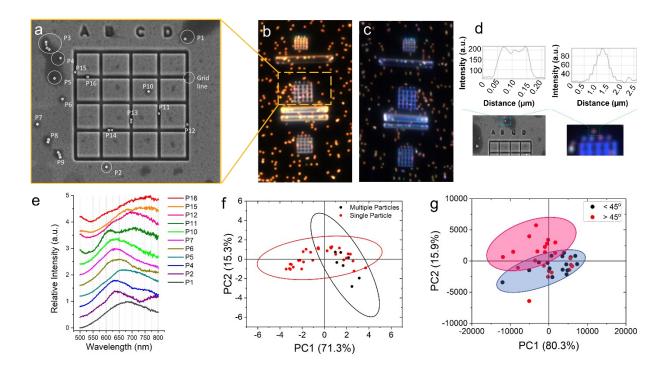


Figure 3. (a) SEM image of the ITO-coated glass substrate patterned using FIB milling. P1-P16 are the nanoparticles marked in the SEM image for which darkfield, hyperspectral image, and scattering spectra are taken; (b) Dark-field optical image of three different grids with several nanocubes on and near them. A subset of this image is shown in (a); (c) Dark-field hyperspectral image of the nanocubes shown in (b); (d) Comparison of the linewidth of pixels across a single nanoparticle as captured in SEM (FWHM ~100 nm) and of the same nanoparticle as it appears in the diffraction-limited hyperspectral dataset image (FWHM ~ 500 nm); (e) Scattering spectra obtained from the hyperspectral images for the particles numbered P1 – P16 in (a); (f) PCA analysis of the single particle spectra as compared to spectra obtained from a cluster of more than one particle; (g) PCA analyses of the scattering spectra for particles with angles  $\theta < 45^{\circ}$  and  $\theta > 45^{\circ}$ .

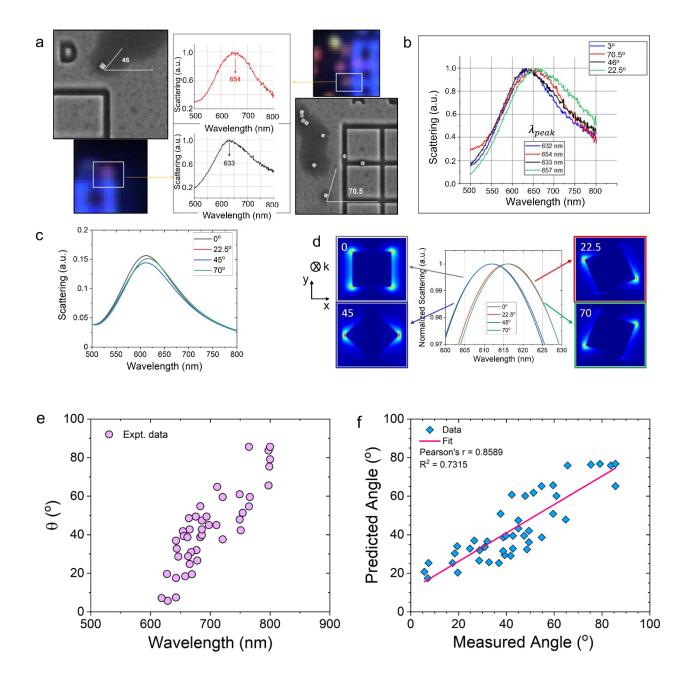


Figure 4. (a) SEM images showing two nanocubes with different orientation. The hyperspectral images of the nanocubes and their corresponding scattering spectra are also shown; (b) Scattering spectra collected from four different nanocubes with orientation,  $\theta = 3^{\circ}$ , 22.5°, 46°, and 70.5°; (c) Scattering spectra obtained using FDTD simulations for nanocubes with orientation  $\theta = 0^{\circ}$ , 22.5°, 45°, and 70° and (d) the corresponding electric field intensity distributions; (e) Scattering peaks obtained from hyperspectral microscopy results and the corresponding measured angles obtained

from the SEM images; **(f)** Correlation between the measured orientation of the nanocubes using SEM images and the predicted orientation of the nanocubes using FDTD simulations for the scattering peaks shown in (e).

#### References

- 1. Ciofani, G., Smart nanoparticles for biomedicine. 2018: Elsevier.
- 2. Dreaden, E.C., et al., *The golden age: gold nanoparticles for biomedicine.* Chemical Society Reviews, 2012. **41**(7): p. 2740-2779.
- 3. Johnson, B.F., Nanoparticles in catalysis. Topics in Catalysis, 2003. 24(1): p. 147-159.
- 4. Peng, H.-I. and B.L. Miller, *Recent advancements in optical DNA biosensors: exploiting the plasmonic effects of metal nanoparticles.* Analyst, 2011. **136**(3): p. 436-447.
- 5. Tsai, C.-S., T.-B. Yu, and C.-T. Chen, *Gold nanoparticle-based competitive colorimetric assay for detection of protein–protein interactions.* Chemical Communications, 2005(34): p. 4273-4275.
- 6. Sergiienko, S., et al., *Nanoparticle–nanoparticle vs. nanoparticle–substrate hot spot contributions to the SERS signal: studying Raman labelled monomers, dimers and trimers.* Physical Chemistry Chemical Physics, 2017. **19**(6): p. 4478-4487.
- 7. Hema, E., et al., A novel synthesis of Zn2+-doped CoFe2O4 spinel nanoparticles: structural, morphological, opto-magnetic and catalytic properties. Journal of Superconductivity and Novel Magnetism, 2015. **28**(8): p. 2539-2552.
- 8. Lessard-Viger, M., et al., FRET enhancement in multilayer core—shell nanoparticles. Nano letters, 2009. **9**(8): p. 3066-3071.
- 9. Feng, L., et al., *Detection of TNT based on conjugated polymer encapsulated in mesoporous silica nanoparticles through FRET.* Chemical Communications, 2012. **48**(38): p. 4633-4635.
- 10. Chen, J.I., Y. Chen, and D.S. Ginger, *Plasmonic nanoparticle dimers for optical sensing of DNA in complex media*. Journal of the American Chemical Society, 2010. **132**(28): p. 9600-9601.
- 11. Nordlander, P., et al., *Plasmon hybridization in nanoparticle dimers.* Nano letters, 2004. **4**(5): p. 899-903.
- 12. Service, R.F., *Nanotechnology takes aim at cancer*. Science, 2005. **310**(5751): p. 1132-1134.
- 13. Xia, Y., Nanomaterials at work in biomedical research. Nature materials, 2008. **7**(10): p. 758-760.
- 14. Mitragotri, S. and J. Lahann, *Physical approaches to biomaterial design.* Nature materials, 2009. **8**(1): p. 15-23.
- 15. Nel, A.E., et al., *Understanding biophysicochemical interactions at the nano–bio interface.* Nature materials, 2009. **8**(7): p. 543-557.
- 16. Wang, Y., et al., Comparison study of gold nanohexapods, nanorods, and nanocages for photothermal cancer treatment. ACS nano, 2013. **7**(3): p. 2068-2077.
- 17. Hu, W., et al., Vertical Orientation Probability Matters for Enhancing Nanoparticle-Macrophage Interaction and Efficient Phagocytosis. Small Methods, 2022: p. 2101601.
- 18. Lou, H.-Y., et al., *Membrane curvature underlies actin reorganization in response to nanoscale surface topography.* Proceedings of the National Academy of Sciences, 2019. **116**(46): p. 23143-23151.
- 19. Champion, J.A. and S. Mitragotri, *Role of target geometry in phagocytosis.* Proceedings of the National Academy of Sciences, 2006. **103**(13): p. 4930-4934.
- Yang, K. and Y.-Q. Ma, *Computer simulation of the translocation of nanoparticles with different shapes across a lipid bilayer*. Nature nanotechnology, 2010. **5**(8): p. 579-583.
- 21. Yang, K., B. Yuan, and Y.-q. Ma, *Influence of geometric nanoparticle rotation on cellular internalization process.* Nanoscale, 2013. **5**(17): p. 7998-8006.
- Herd, H., et al., *Nanoparticle geometry and surface orientation influence mode of cellular uptake.* ACS nano, 2013. **7**(3): p. 1961-1973.
- 23. Vácha, R., F.J. Martinez-Veracoechea, and D. Frenkel, *Receptor-mediated endocytosis of nanoparticles of various shapes*. Nano letters, 2011. **11**(12): p. 5391-5395.

- 24. He, X., K. Wang, and Z. Cheng, *In vivo near-infrared fluorescence imaging of cancer with nanoparticle-based probes.* Wiley Interdisciplinary Reviews: Nanomedicine and Nanobiotechnology, 2010. **2**(4): p. 349-366.
- 25. Liu, Y., Y.-c. Tseng, and L. Huang, *Biodistribution studies of nanoparticles using fluorescence imaging: a qualitative or quantitative method?* Pharmaceutical research, 2012. **29**(12): p. 3273-3277.
- 26. Pal, S., et al., Surface Spin Disorder in Fe \$ \_ {3} \$ O \$ \_ {4} \$ Nanoparticles Probed by Electron Magnetic Resonance Spectroscopy and Magnetometry. IEEE transactions on magnetics, 2007. 43(6): p. 3091-3093.
- 27. Monti, O.L., J.T. Fourkas, and D.J. Nesbitt, *Diffraction-limited photogeneration and characterization of silver nanoparticles*. The Journal of Physical Chemistry B, 2004. **108**(5): p. 1604-1612.
- 28. Seydack, M., *Nanoparticle labels in immunosensing using optical detection methods.* Biosensors and bioelectronics, 2005. **20**(12): p. 2454-2469.
- 29. O'Neal, D.P., et al., *Photo-thermal tumor ablation in mice using near infrared-absorbing nanoparticles*. Cancer letters, 2004. **209**(2): p. 171-176.
- 30. Tcherniak, A., et al., *One-photon plasmon luminescence and its application to correlation spectroscopy as a probe for rotational and translational dynamics of gold nanorods.* The Journal of Physical Chemistry C, 2011. **115**(32): p. 15938-15949.
- 31. Wang, H., et al., *In vitro and in vivo two-photon luminescence imaging of single gold nanorods.* Proceedings of the National Academy of Sciences, 2005. **102**(44): p. 15752-15756.
- 32. Hashimoto, S., D. Werner, and T. Uwada, *Studies on the interaction of pulsed lasers with plasmonic gold nanoparticles toward light manipulation, heat management, and nanofabrication.* Journal of Photochemistry and Photobiology C: Photochemistry Reviews, 2012. **13**(1): p. 28-54.
- 33. Li, T., et al., *Three-dimensional orientation sensors by defocused imaging of gold nanorods through an ordinary wide-field microscope*. ACS nano, 2012. **6**(2): p. 1268-1277.
- 34. Sönnichsen, C. and A.P. Alivisatos, *Gold nanorods as novel nonbleaching plasmon-based orientation sensors for polarized single-particle microscopy.* Nano letters, 2005. **5**(2): p. 301-304.
- 35. Biswas, S., et al., *Orientation sensing with color using plasmonic gold nanorods and assemblies.* The Journal of Physical Chemistry Letters, 2012. **3**(18): p. 2568-2574.
- 36. Huang, Y. and D.-H. Kim, *Dark-field microscopy studies of polarization-dependent plasmonic resonance of single gold nanorods: rainbow nanoparticles.* Nanoscale, 2011. **3**(8): p. 3228-3232.
- 37. Mehta, N., et al., *Dark-field hyperspectral imaging for label free detection of nano-bio-materials.*Wiley Interdisciplinary Reviews: Nanomedicine and Nanobiotechnology, 2021. **13**(1): p. e1661.
- 38. Hu, J., et al., *Single-nanoparticle orientation sensing by deep learning*. ACS central science, 2020. **6**(12): p. 2339-2346.
- 39. Kawata, S., Y. Inouye, and P. Verma, *Plasmonics for near-field nano-imaging and superlensing*. Nature photonics, 2009. **3**(7): p. 388-394.
- 40. Weast, R.C., M.J. Astle, and W.H. Beyer, *CRC handbook of chemistry*. Physics, CRC Press, Boca Raton 1988, D, 1981. **151**.
- 41. Khlebtsov, N., L. Trachuk, and A. Mel'nikov, *The effect of the size, shape, and structure of metal nanoparticles on the dependence of their optical properties on the refractive index of a disperse medium.* Optics and spectroscopy, 2005. **98**(1): p. 77-83.
- 42. Barnes, W.L., A. Dereux, and T.W. Ebbesen, *Surface plasmon subwavelength optics.* nature, 2003. **424**(6950): p. 824-830.
- 43. Wu, C., et al., Surface modification of indium tin oxide by plasma treatment: An effective method to improve the efficiency, brightness, and reliability of organic light emitting devices. Applied Physics Letters, 1997. **70**(11): p. 1348-1350.

- 44. Gautam, R., et al., *Review of multidimensional data processing approaches for Raman and infrared spectroscopy.* EPJ Techniques and Instrumentation, 2015. **2**(1): p. 1-38.
- 45. Beattie, J.R. and F.W. Esmonde-White, *Exploration of principal component analysis: deriving principal component analysis visually using spectra*. Applied Spectroscopy, 2021. **75**(4): p. 361-375.
- 46. Mehta, N., et al., *Multimodal Label-Free Monitoring of Adipogenic Stem Cell Differentiation Using Endogenous Optical Biomarkers*. Advanced Functional Materials, 2021. **31**(43): p. 2103955.
- 47. Ikponmwoba, E., et al., A Machine Learning Framework for Detecting COVID-19 Infection Using Surface-Enhanced Raman Scattering. Biosensors, 2022. **12**(8): p. 589.
- 48. Mukaka, M.M., *A guide to appropriate use of correlation coefficient in medical research.* Malawi medical journal, 2012. **24**(3): p. 69-71.
- 49. Adler, J. and I. Parmryd, *Quantifying colocalization by correlation: the Pearson correlation coefficient is superior to the Mander's overlap coefficient.* Cytometry Part A, 2010. **77**(8): p. 733-742.
- 50. Dunn, K.W., M.M. Kamocka, and J.H. McDonald, *A practical guide to evaluating colocalization in biological microscopy.* American Journal of Physiology-Cell Physiology, 2011. **300**(4): p. C723-C742.